

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110518\
 Data File : VW006645.D
 Acq On : 05 Nov 2018 19:07
 Operator : SY/AP
 Sample : J5700-05
 Misc : 6.43G/5ML/MSVOA W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SI-5

Quant Time: Nov 06 03:08:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 01 03:48:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	196029	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	282263	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	247818	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	109561	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	76443	45.37	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.74%	
35) Dibromofluoromethane	7.88	113	76324	43.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.18%	
50) Toluene-d8	10.33	98	251040	37.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	74.46%	
62) 4-Bromofluorobenzene	12.62	95	79890	32.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	65.36%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110518\
Data File : VW006645.D
Acq On : 05 Nov 2018 19:07
Operator : SY/AP
Sample : J5700-05
Misc : 6.43G/5ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SI-5

Quant Time: Nov 06 03:08:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 01 03:48:08 2018
Response via : Initial Calibration

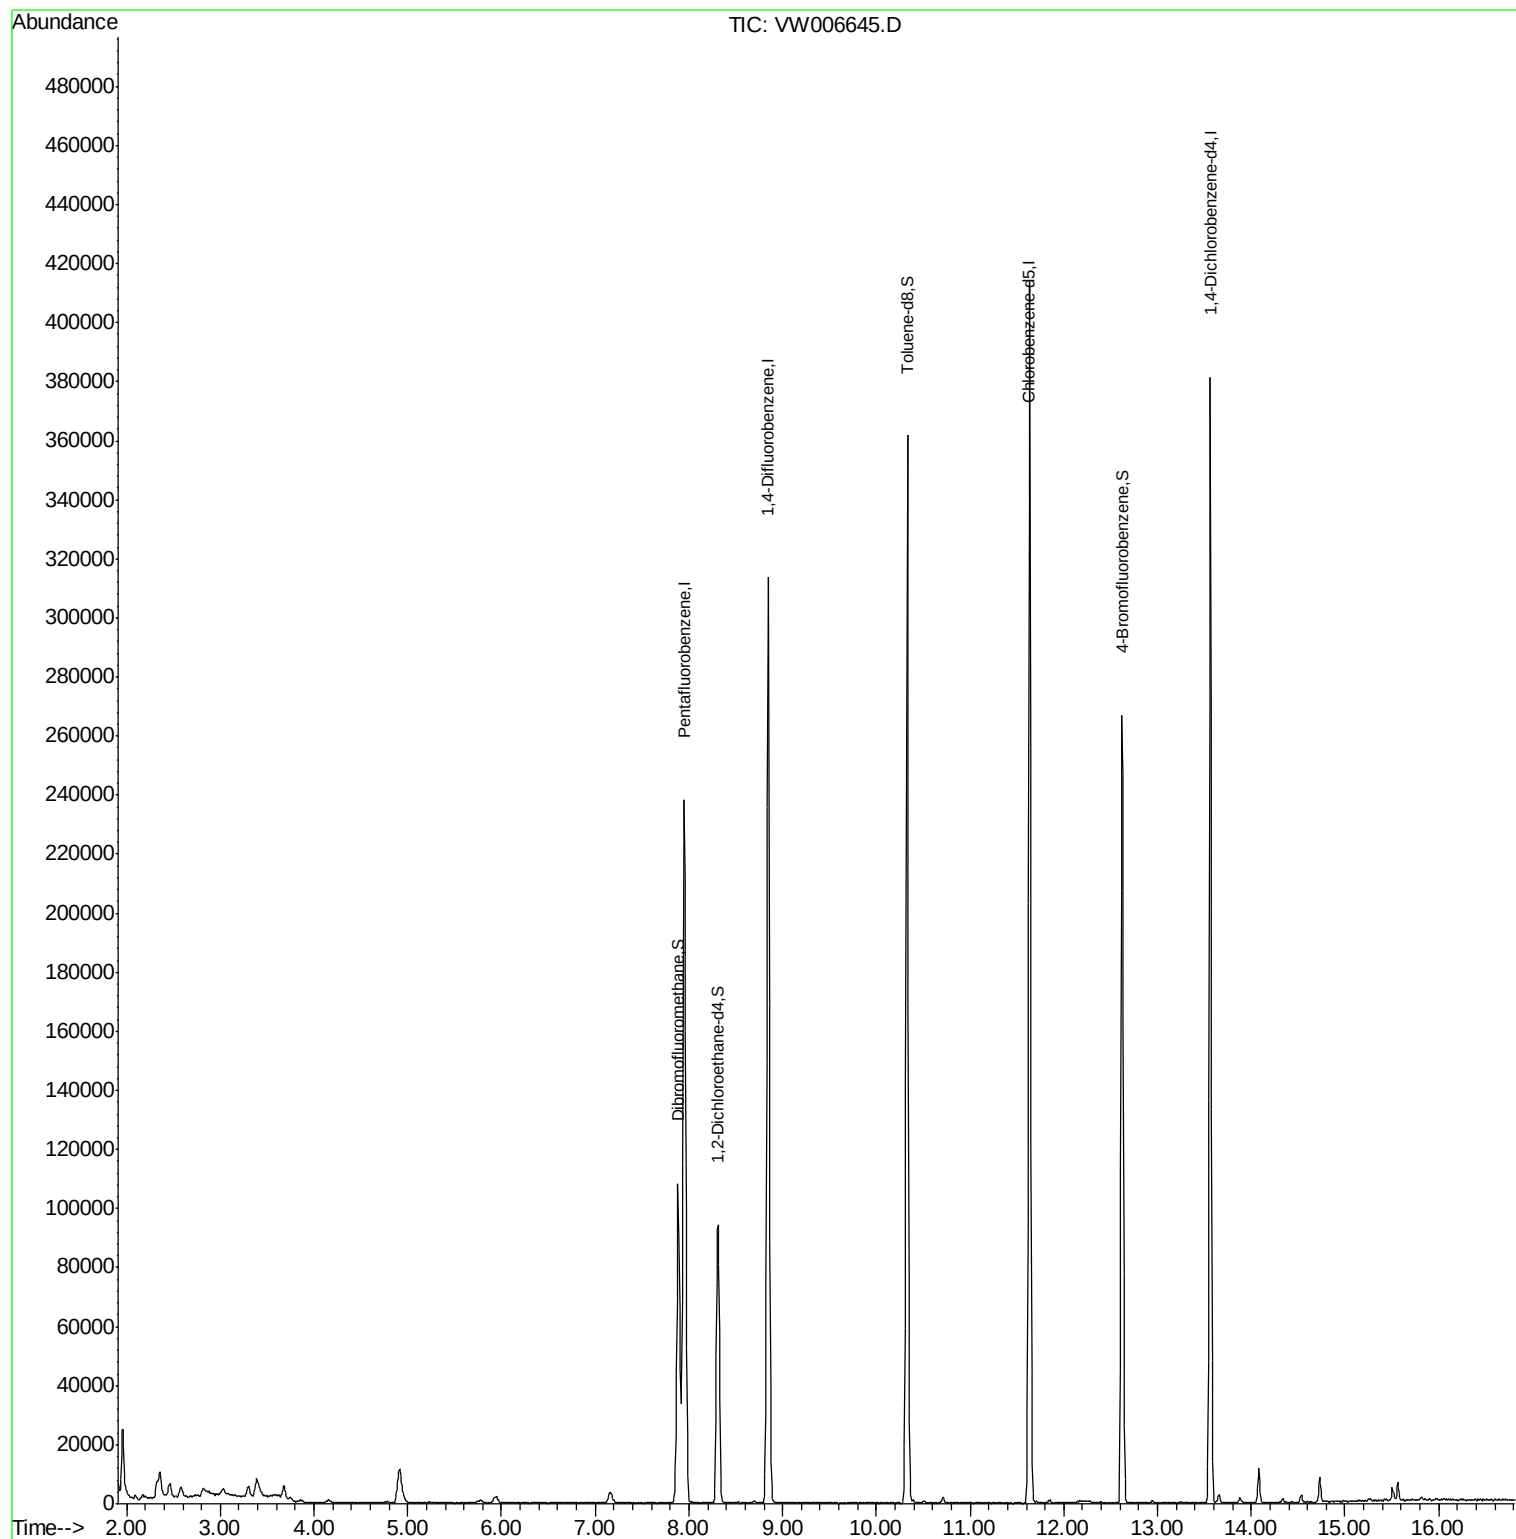

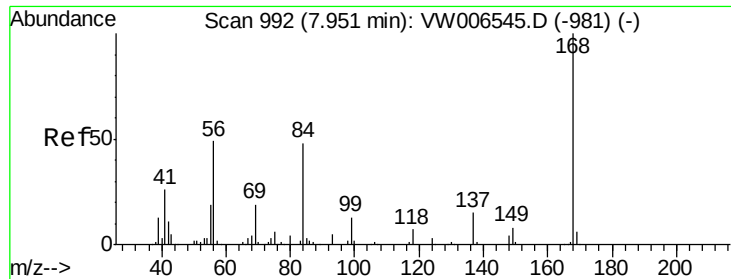

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006645.D

Acq: 05 Nov 2018 19:07

Instrument :

MSVOA_W

ClientSampled :


SI-5

Tot Ion:168 Resp: 196029

Ion Ratio Lower Upper

168 100




99 46.8 37.4 56.0

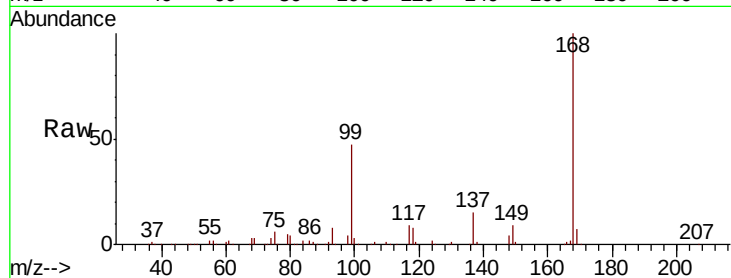

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

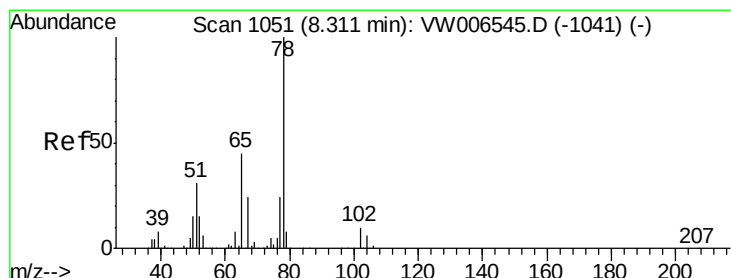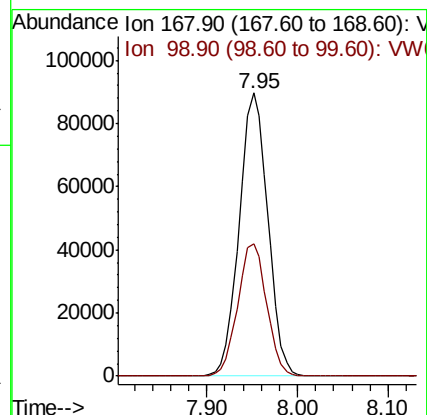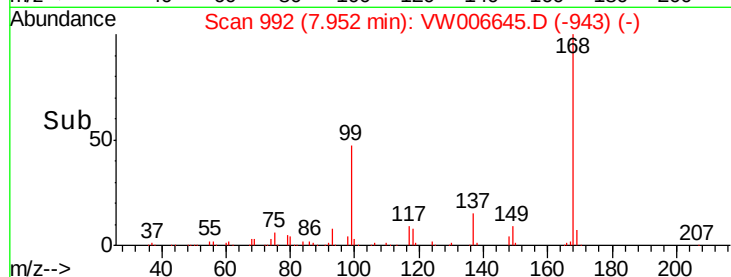

#33

1,2-Dichloroethane-d4

Concen: 45.365 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.01 min

Lab File: VW006645.D


Acq: 05 Nov 2018 19:07

Tgt Ion: 65 Resp: 76443

Ion Ratio Lower Upper

65 100



67 50.9 0.0 104.4

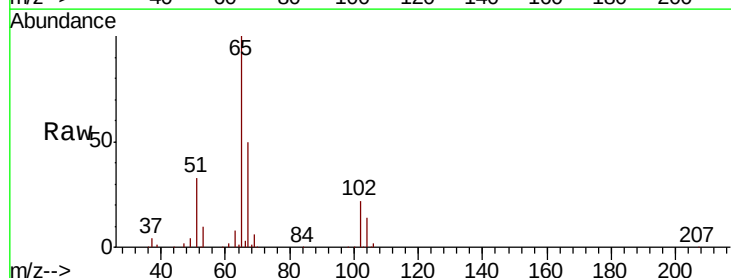


Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

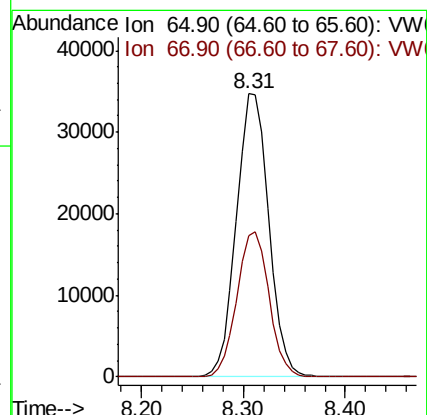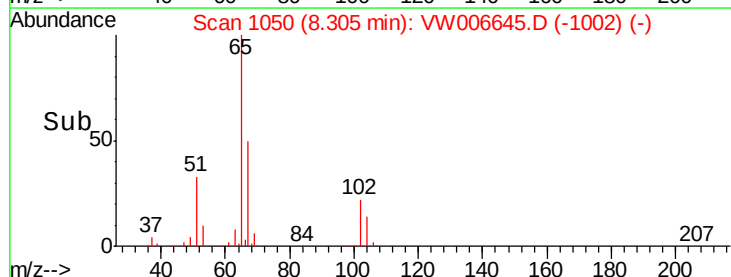


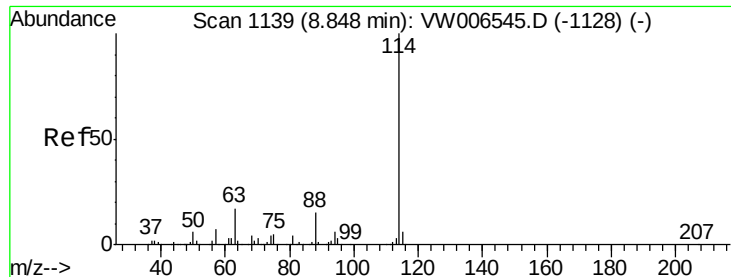




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006645.D
 Acq: 05 Nov 2018 19:07

Instrument :
 MSVOA_W
 ClientSampleId :
 SI-5

Tot Ion:114	Resp:	282263
Ion Ratio	Lower	Upper
114 100		
63 18.0	0.0	34.4
88 14.0	0.0	29.0

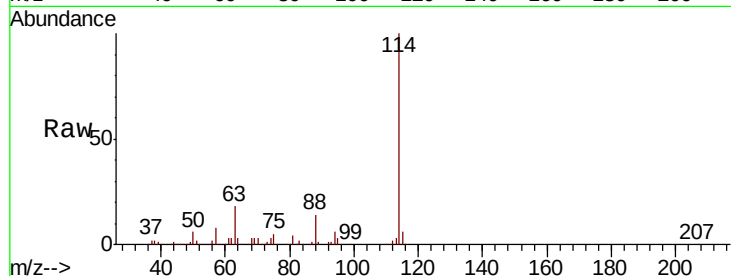


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

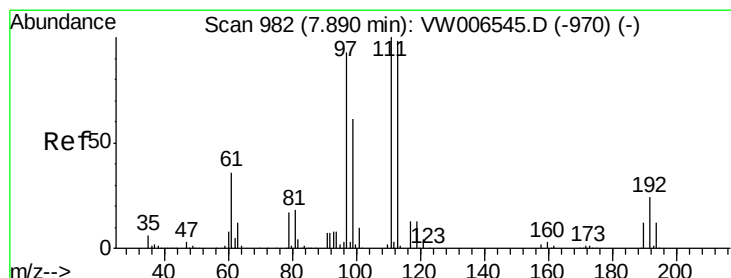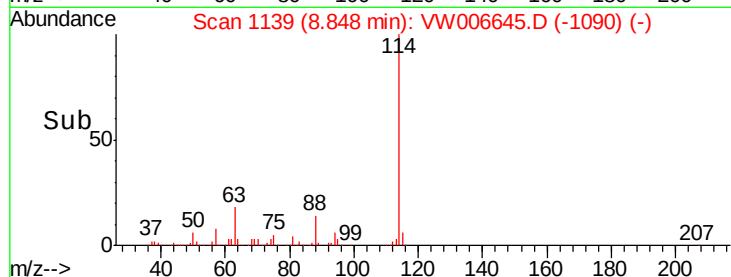
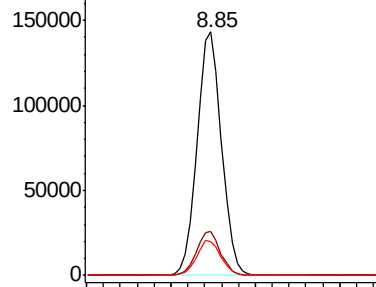



#35
 Dibromofluoromethane
 Concen: 43.086 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.01 min
 Lab File: VW006645.D
 Acq: 05 Nov 2018 19:07

Tgt Ion:113	Resp:	76324
Ion Ratio	Lower	Upper
113 100		
111 100.5	82.2	123.2
192 23.3	19.0	28.6

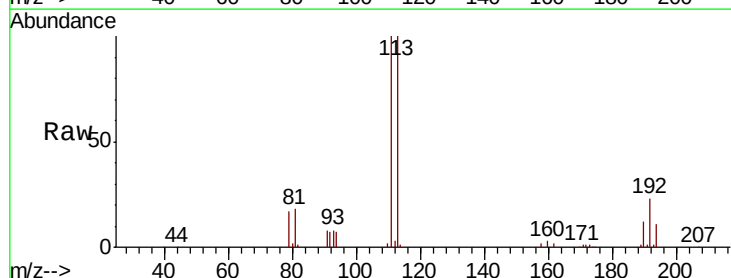

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

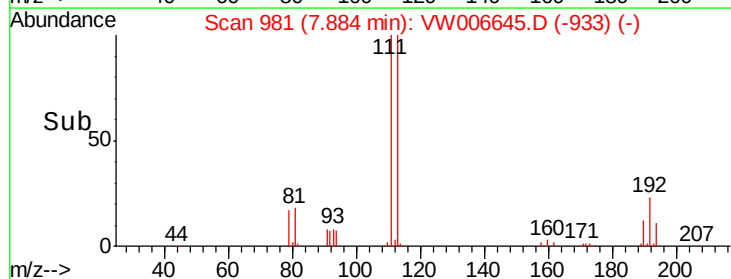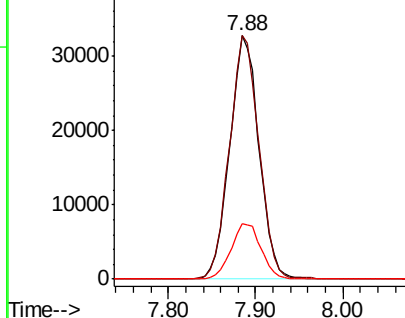

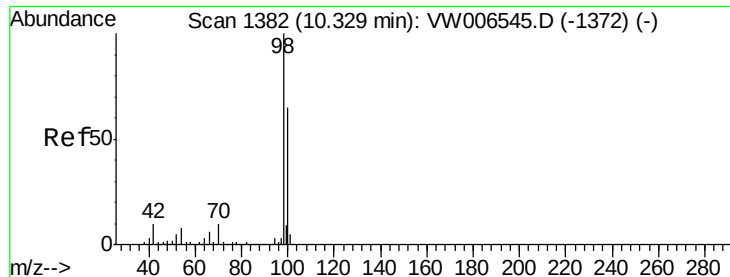

#50

Toluene-d8

Concen: 37.227 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW006645.D

Acq: 05 Nov 2018 19:07

Instrument :

MSVOA_W

ClientSampleId :





SI-5

Tot Ion: 98 Resp: 251040

Ion Ratio Lower Upper

98 100

100 64.5 51.6 77.4

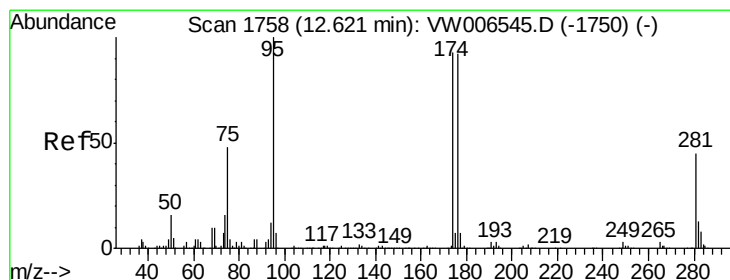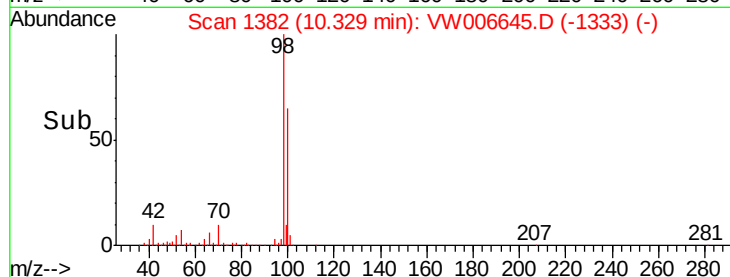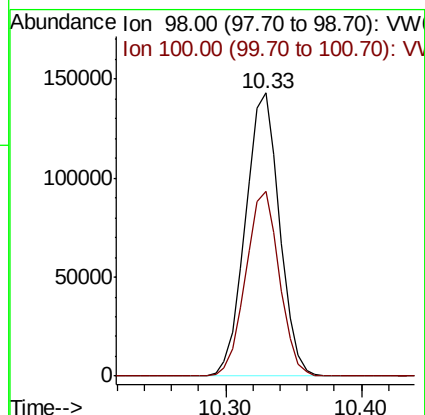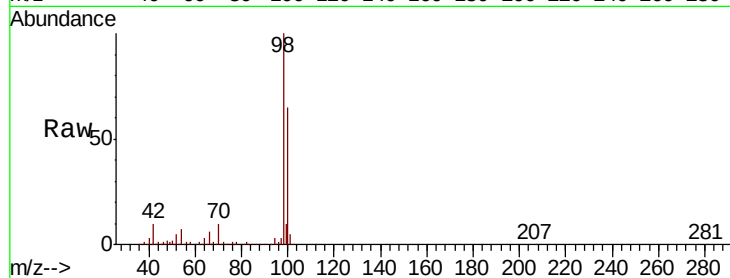

#62

4-Bromofluorobenzene

Concen: 32.678 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006645.D

Acq: 05 Nov 2018 19:07




Tgt Ion: 95 Resp: 79890


Ion Ratio Lower Upper

95 100

174 99.5 0.0 192.4

176 97.1 0.0 187.4

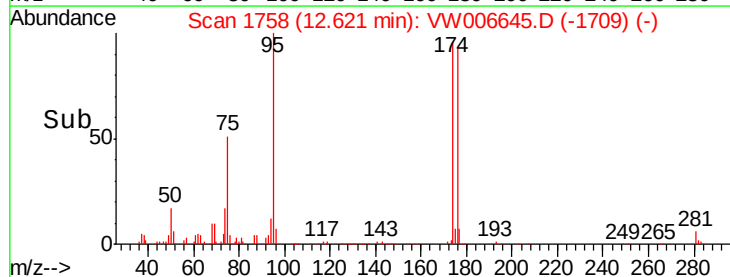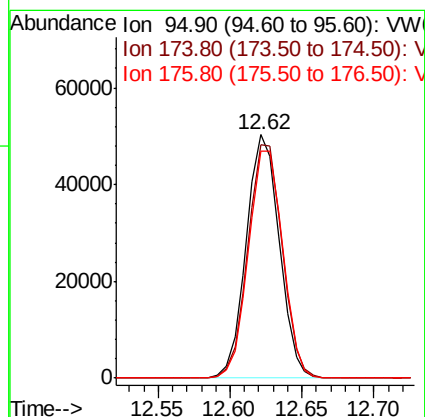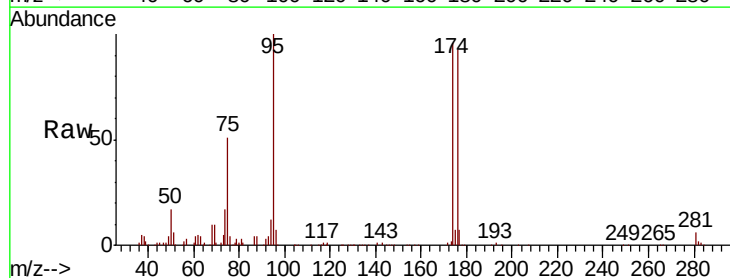


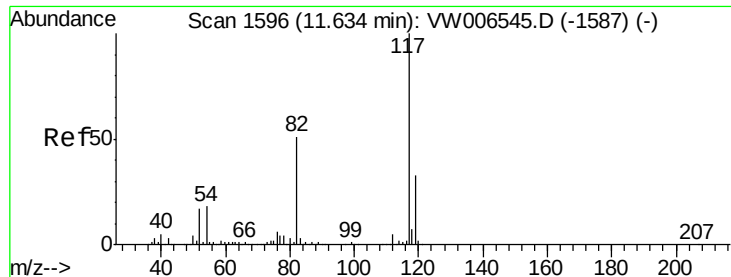

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW006645.D
Acq: 05 Nov 2018 19:07

Instrument :
MSVOA_W
ClientSampleId :
SI-5

Tot Ion	Ratio	Lower	Upper
117	100		
82	51.2	40.8	61.2
119	32.2	26.1	39.1



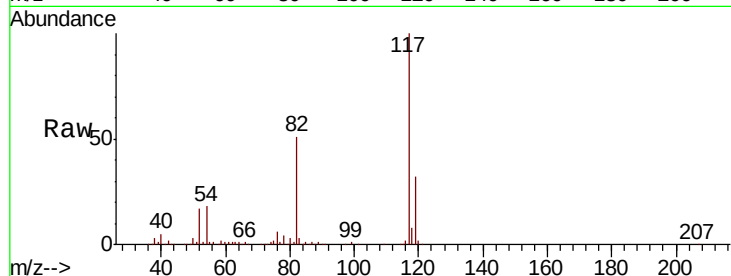


Abundance

Ion 116.90 (116.60 to 117.60): V


Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

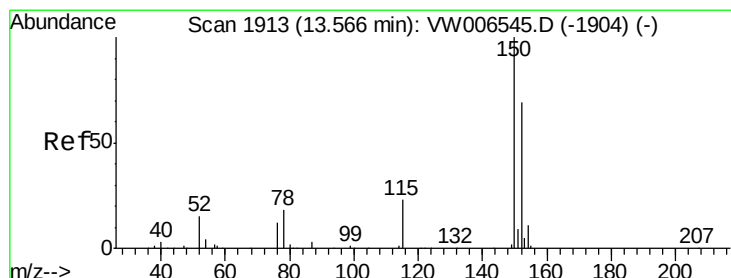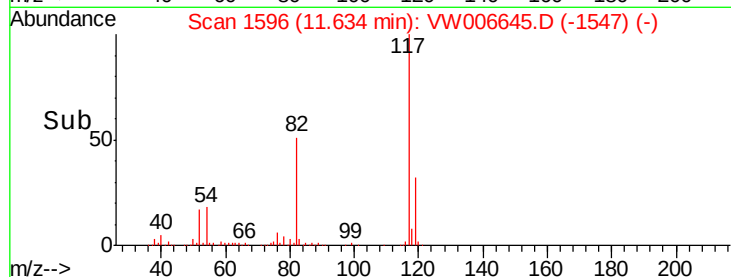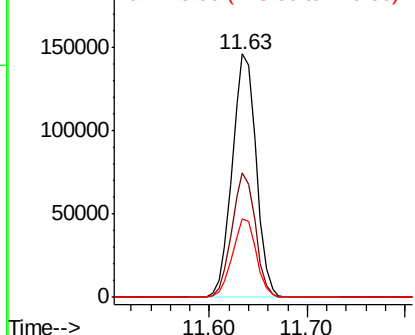

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. 0.00 min
Lab File: VW006645.D
Acq: 05 Nov 2018 19:07

Tgt Ion	Ratio	Lower	Upper
152	100		
115	52.8	26.6	79.8
150	157.2	0.0	344.6

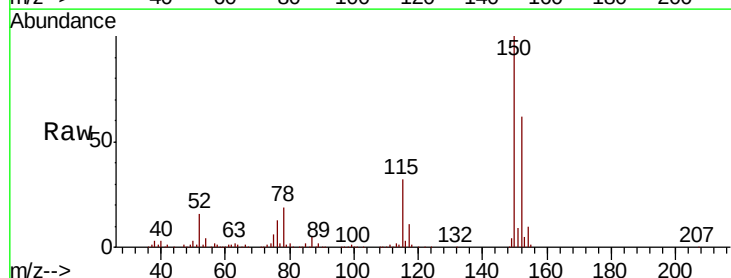

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

