


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110518\
 Data File : VW006625.D
 Acq On : 05 Nov 2018 09:58
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Title : SW846 8260
 Last Update : Thu Nov 01 03:48:08 2018

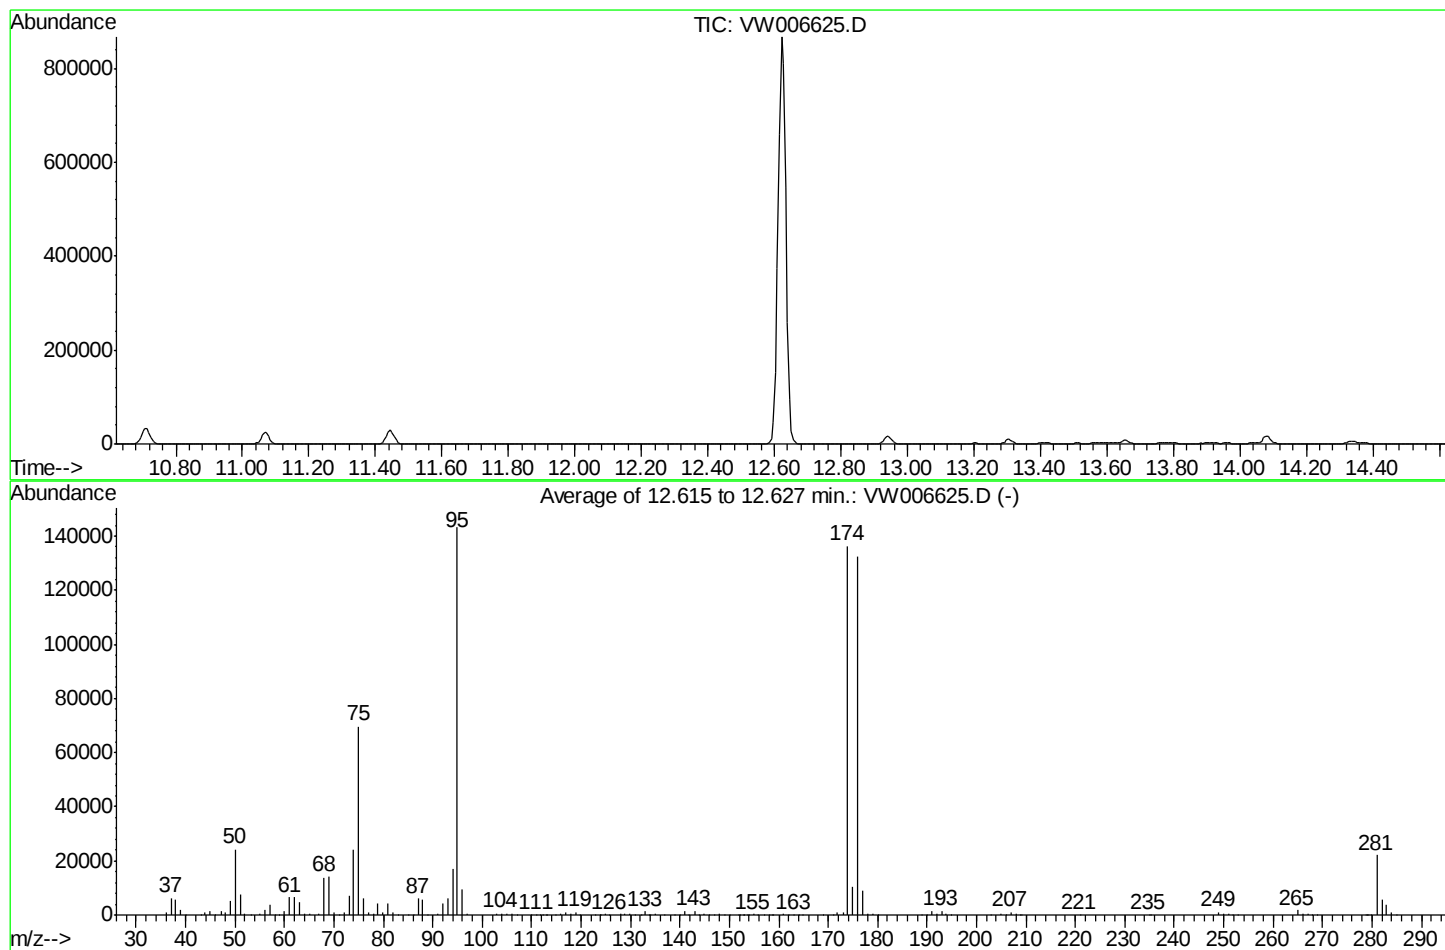

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	24258	PASS
75	95	30	60	48.6	69605	PASS
95	95	100	100	100.0	143240	PASS
96	95	5	9	6.7	9634	PASS
173	174	0.00	2	0.8	1026	PASS
174	95	50	100	95.1	136261	PASS
175	174	5	9	7.7	10426	PASS
176	174	95	101	97.1	132330	PASS
177	176	5	9	7.0	9233	PASS