


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110520\
 Data File : VW017085.D
 Acq On : 05 Nov 2020 08:30
 Operator : SY/VA
 Sample : BFB29
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB29

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Title : VOC Analysis
 Last Update : Sat Nov 07 04:26:24 2020

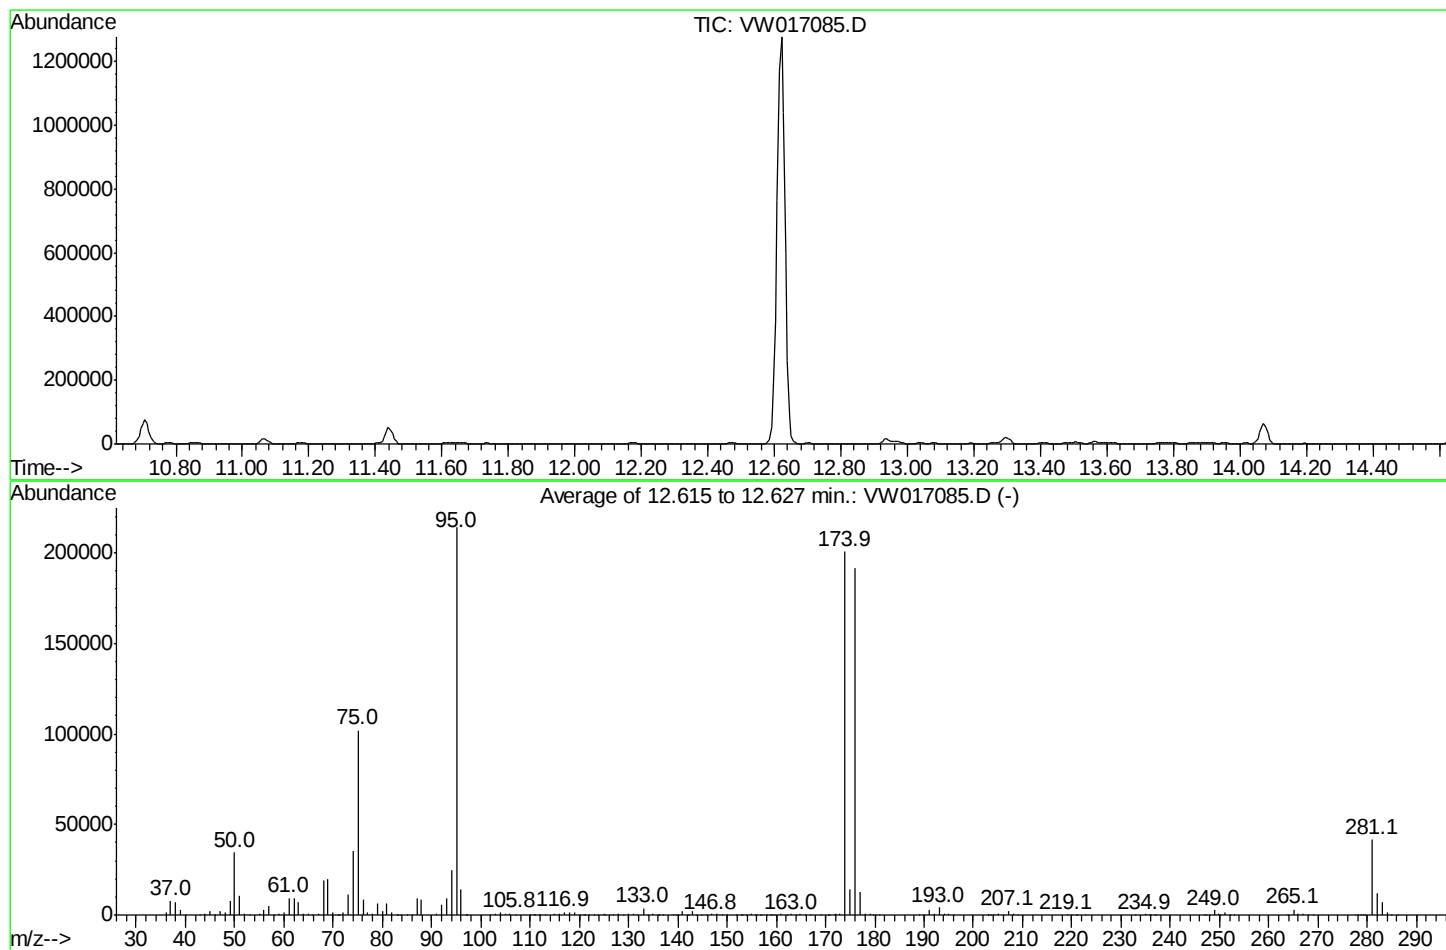

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	34354	PASS
75	95	30	80	47.6	101805	PASS
95	95	100	100	100.0	214080	PASS
96	95	5	9	6.7	14290	PASS
173	174	0.00	2	0.3	682	PASS
174	95	50	120	93.7	200554	PASS
175	174	5	9	7.1	14149	PASS
176	174	95	101	95.4	191424	PASS
177	176	5	9	6.7	12736	PASS

Scan 1749 (12.566 min): VW017085.D
BFB29

m/z	Abundance
40.00	121.0
41.00	78.0
44.00	135.0
56.80	65.0
169.10	58.0
207.10	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	1618.0
37.00	8445.0
38.00	7987.0
39.00	2589.0
40.10	185.0
40.90	66.0
43.00	249.0
43.90	1183.0
45.00	2079.0
45.90	238.0
47.00	2347.0
48.00	1179.0
49.00	8441.0
50.00	34560.0
51.00	10895.0
52.00	454.0
53.10	86.0
55.00	566.0
56.00	3045.0
57.00	5213.0
58.00	288.0
59.00	735.0
60.00	1720.0
61.00	9116.0
62.00	9378.0
63.00	6495.0
64.10	799.0
65.00	400.0
65.80	83.0
67.00	636.0
68.00	19616.0
69.00	19616.0
70.00	1646.0
71.00	173.0
72.00	1243.0
73.00	12711.0
74.00	35320.0
75.00	103664.0
76.00	9157.0
77.00	1409.0
78.00	849.0
79.00	6064.0
79.90	1631.0
80.90	6261.0
81.90	1436.0
83.10	178.0
83.60	107.0
85.10	87.0
86.00	365.0
87.00	9035.0
87.90	8227.0
90.90	836.0
92.00	5449.0
93.00	9213.0
94.00	23600.0
95.00	210432.0
96.00	14867.0
97.00	405.0
101.90	81.0
103.00	1189.0
103.90	1032.0
104.90	418.0
105.90	823.0
107.00	273.0
110.00	414.0
110.80	339.0
111.80	389.0
112.90	188.0
114.90	557.0
115.90	758.0
116.90	1762.0
118.00	1189.0
118.90	1839.0
120.10	102.0
120.80	240.0
121.90	73.0
123.00	51.0
123.80	154.0
125.00	1173.0
127.90	679.0
128.80	368.0
129.90	749.0
130.90	447.0
131.90	162.0
133.00	5831.0
135.00	781.0
135.80	193.0
136.90	377.0
139.00	90.0
140.00	197.0
141.00	1944.0
141.80	219.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

142.90	2210.0
143.80	138.0
144.90	348.0
145.90	415.0
146.80	870.0
148.00	571.0
148.90	367.0
149.80	202.0
152.00	94.0
153.10	136.0
153.70	112.0
155.00	477.0
155.90	200.0
156.90	443.0
158.00	102.0
158.80	259.0
161.00	480.0
162.10	125.0
163.00	779.0
163.90	222.0
165.00	626.0
165.90	109.0
166.90	63.0
168.90	60.0
170.50	57.0
171.90	791.0
172.90	2048.0
173.90	182720.0
175.00	12414.0
175.90	172480.0
177.00	11834.0
178.00	743.0
179.10	1267.0
180.00	184.0
180.90	245.0
189.00	482.0
189.90	162.0
191.00	4375.0
192.00	997.0
193.00	6211.0
194.10	1099.0
194.90	550.0
196.10	80.0
202.90	598.0
203.60	137.0
205.00	1200.0
206.10	436.0
207.00	4018.0
208.10	929.0
209.10	385.0
219.10	131.0
221.00	183.0
222.80	54.0
232.80	73.0
234.90	561.0
236.10	176.0
236.90	126.0
246.90	59.0
247.20	56.0
247.90	61.0
249.00	3546.0
249.90	975.0
251.00	1664.0
252.10	413.0
253.00	391.0
265.10	4182.0
266.00	1420.0
267.00	1273.0
267.90	177.0
269.10	130.0
278.10	164.0
278.70	227.0
279.20	326.0
281.00	60808.0
282.10	17688.0
283.10	9527.0
284.00	1732.0
285.00	611.0
286.10	112.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	1479.0
37.00	9094.0
38.00	7580.0
39.00	2959.0
39.90	241.0
42.90	174.0
44.00	1381.0
45.00	2117.0
47.00	2434.0
48.00	1155.0
49.00	7978.0
50.00	38624.0
51.00	12396.0
52.00	527.0
53.20	55.0
55.00	757.0
56.00	3131.0
57.00	5587.0
58.00	198.0
59.10	468.0
60.00	1853.0
61.00	10409.0
62.00	10263.0
63.00	7549.0
64.00	805.0
65.00	352.0
65.80	72.0
67.00	719.0
68.00	21992.0
69.00	22568.0
70.00	1777.0
72.00	1208.0
73.00	12289.0
74.00	39504.0
75.00	110032.0
76.10	9051.0
77.00	1440.0
77.90	869.0
78.90	6671.0
79.90	2211.0
80.90	7214.0
81.90	1565.0
83.10	194.0
83.60	115.0
85.00	71.0
85.80	324.0
87.00	9928.0
87.90	10288.0
91.00	1036.0
92.00	6338.0
93.00	10021.0
94.00	27952.0
95.00	236224.0
96.00	16262.0
97.00	569.0
101.80	59.0
102.90	572.0
103.90	1359.0
104.90	536.0
105.80	953.0
107.00	314.0
109.90	273.0
110.60	261.0
111.10	363.0
112.10	267.0
113.00	207.0
114.80	396.0
115.90	921.0
116.90	1587.0
117.90	1203.0
118.90	1474.0
120.00	97.0
121.00	108.0
121.80	107.0
122.90	100.0
123.70	181.0
125.00	1200.0
126.70	55.0
127.90	782.0
128.80	380.0
129.90	1022.0
130.90	430.0
132.00	116.0
133.00	3440.0
133.90	762.0
134.90	543.0
136.10	134.0
136.90	435.0
139.00	125.0
140.00	170.0
140.90	2258.0
141.90	277.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

142.90	2408.0
143.90	155.0
144.90	363.0
145.80	382.0
146.90	663.0
147.90	647.0
148.80	346.0
149.90	306.0
151.80	121.0
152.80	294.0
153.80	155.0
154.80	695.0
155.60	126.0
156.70	309.0
157.10	378.0
158.10	140.0
159.00	395.0
160.90	551.0
162.10	93.0
163.00	551.0
163.90	80.0
164.80	438.0
168.90	66.0
170.50	80.0
172.10	724.0
173.90	220928.0
175.00	16243.0
175.90	209472.0
176.90	14719.0
178.00	697.0
178.90	940.0
179.70	157.0
181.00	132.0
189.00	330.0
191.00	3253.0
192.10	786.0
193.00	4211.0
194.00	586.0
194.90	495.0
203.10	462.0
204.00	129.0
205.10	873.0
206.00	245.0
207.10	2397.0
208.10	506.0
208.90	276.0
219.10	129.0
220.00	67.0
221.10	172.0
232.90	108.0
235.00	398.0
235.70	106.0
236.10	117.0
237.10	92.0
246.90	59.0
249.00	2823.0
249.80	527.0
250.10	543.0
251.10	1159.0
252.00	344.0
253.10	114.0
263.80	62.0
265.10	2822.0
266.00	812.0
267.10	685.0
267.90	140.0
268.90	71.0
277.70	89.0
278.50	74.0
279.00	201.0
281.10	43336.0
282.10	12118.0
283.10	7467.0
284.10	1509.0
284.90	284.0
286.00	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	1161.0
37.00	6665.0
38.00	5656.0
39.10	2471.0
40.00	255.0
43.10	86.0
44.00	967.0
45.00	1199.0
46.10	93.0
47.00	2114.0
48.00	1063.0
49.00	6338.0
50.00	29880.0
51.00	9060.0
52.10	441.0
55.00	580.0
56.00	2623.0
57.00	4318.0
58.10	211.0
58.90	171.0
60.10	1632.0
61.00	8258.0
62.00	7748.0
63.00	6423.0
64.10	532.0
65.10	396.0
67.00	435.0
68.00	16366.0
69.00	17776.0
70.00	1180.0
71.20	125.0
72.00	1129.0
73.00	8554.0
74.00	30776.0
75.00	91720.0
76.00	7807.0
77.00	1055.0
78.00	807.0
78.90	5819.0
80.00	1628.0
80.90	5966.0
81.90	1353.0
82.80	125.0
86.00	299.0
87.00	7819.0
88.00	8005.0
90.90	794.0
92.00	5413.0
93.00	8273.0
94.00	22888.0
95.00	195584.0
96.00	11742.0
97.20	253.0
102.90	315.0
103.90	1010.0
105.00	334.0
105.90	664.0
107.00	180.0
110.00	180.0
110.80	276.0
111.80	209.0
113.00	210.0
114.80	312.0
115.90	861.0
116.90	1344.0
118.00	910.0
119.00	1227.0
119.90	86.0
122.90	118.0
123.90	174.0
125.20	518.0
126.00	220.0
126.80	59.0
127.80	706.0
128.90	312.0
129.90	739.0
131.00	378.0
131.80	100.0
132.90	1481.0
134.90	577.0
135.90	85.0
136.90	301.0
139.00	85.0
139.70	188.0
141.00	2217.0
142.20	353.0
142.90	2291.0
143.80	152.0
145.00	215.0
145.80	319.0
146.90	339.0
147.90	436.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

148.80	288.0
150.00	278.0
151.90	99.0
152.90	176.0
153.80	108.0
155.00	414.0
156.00	183.0
157.00	327.0
158.00	110.0
159.00	282.0
159.70	86.0
160.90	506.0
162.10	53.0
163.00	263.0
163.80	56.0
164.90	298.0
168.80	57.0
170.70	92.0
172.10	591.0
173.90	198016.0
174.90	13792.0
175.90	192320.0
177.00	11656.0
178.00	421.0
178.90	468.0
180.00	117.0
181.00	93.0
188.90	97.0
191.00	1593.0
192.00	238.0
193.00	1898.0
194.10	347.0
194.90	267.0
203.00	222.0
205.00	432.0
205.90	106.0
207.00	1191.0
208.00	225.0
208.90	156.0
219.10	112.0
220.80	58.0
234.90	184.0
235.90	66.0
237.00	62.0
247.20	51.0
248.90	1488.0
250.00	191.0
251.00	568.0
251.90	276.0
265.10	1822.0
266.10	376.0
267.00	538.0
267.90	61.0
278.70	63.0
279.40	93.0
281.00	20728.0
282.10	5485.0
283.00	3359.0
284.10	605.0
285.00	210.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29