
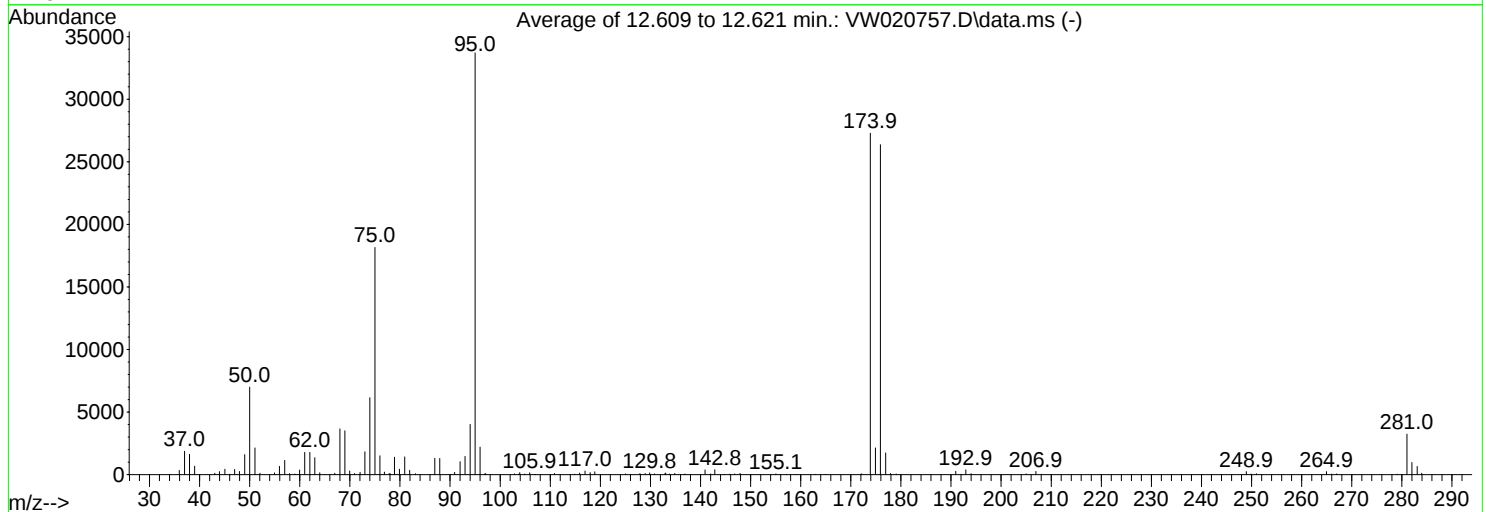


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110521\
Data File : VW020757.D
Acq On : 04 Nov 2021 12:39
Operator : SY/VA
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W110521S.M
Title : SW846 8260
Last Update : Thu Nov 04 19:17:56 2021

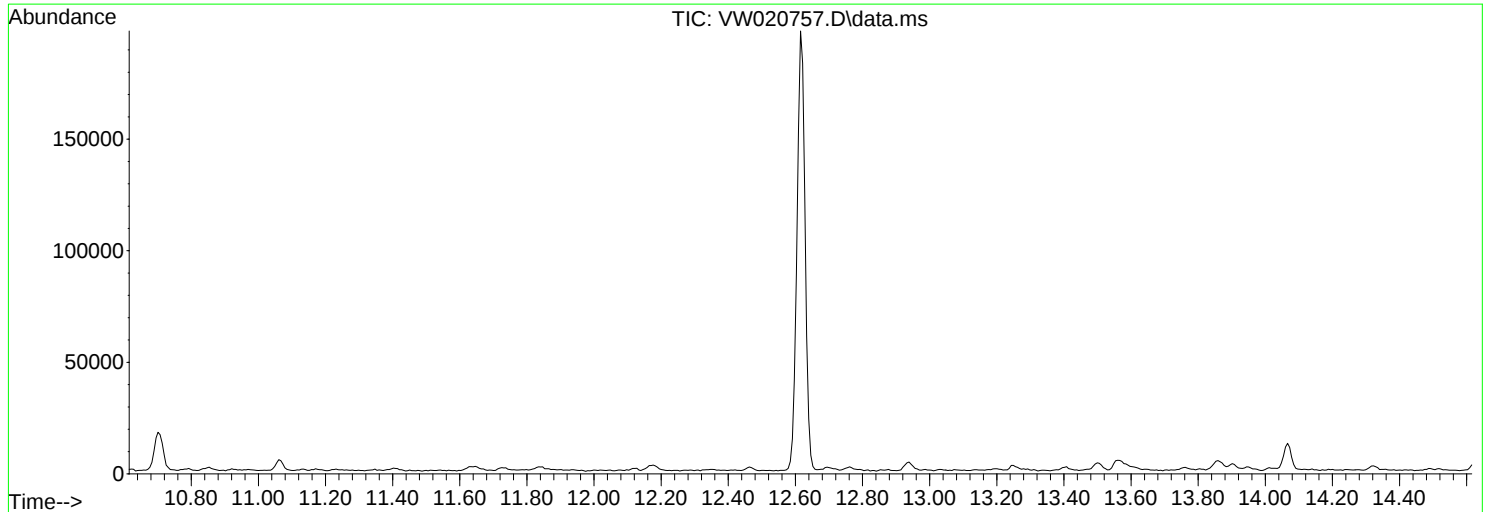

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1746

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	6997	PASS
75	95	30	60	53.9	18161	PASS
95	95	100	100	100.0	33709	PASS
96	95	5	9	6.5	2194	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.9	27283	PASS
175	174	5	9	7.9	2143	PASS
176	174	95	101	96.6	26368	PASS
177	176	5	9	6.6	1735	PASS