

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110524\
 Data File : VW030931.D
 Acq On : 05 Nov 2024 12:14
 Operator : SY/MD
 Sample : P4581-07
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 06 00:12:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 06 00:11:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	475861	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	458177	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	204394	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	161252	20.661	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.640%
7) Chloroethane-d5	2.899	69	128370	21.446	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	4.021	65	74800	23.227	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.920%
21) 2-Butanone-d5	7.075	46	73563	57.276	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.560%
24) Chloroform-d	7.648	84	340902	24.301	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	8.300	65	180820	25.924	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.680%
32) Benzene-d6	8.276	84	688919	24.203	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	9.270	67	204554	24.378	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.520%
41) Toluene-d8	10.324	98	623876	24.436	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.760%
43) trans-1,3-Dichloroprop...	10.574	79	82616	24.290	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.160%
47) 2-Hexanone-d5	10.922	63	62550	57.518	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	156953	26.848	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	199915	26.851	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.400%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	5441	0.493	ug/L	Qvalue # 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110524\
Data File : VW030931.D
Acq On : 05 Nov 2024 12:14
Operator : SY/MD
Sample : P4581-07
Misc : 5.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 06 00:12:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 06 00:11:36 2024
Response via : Initial Calibration

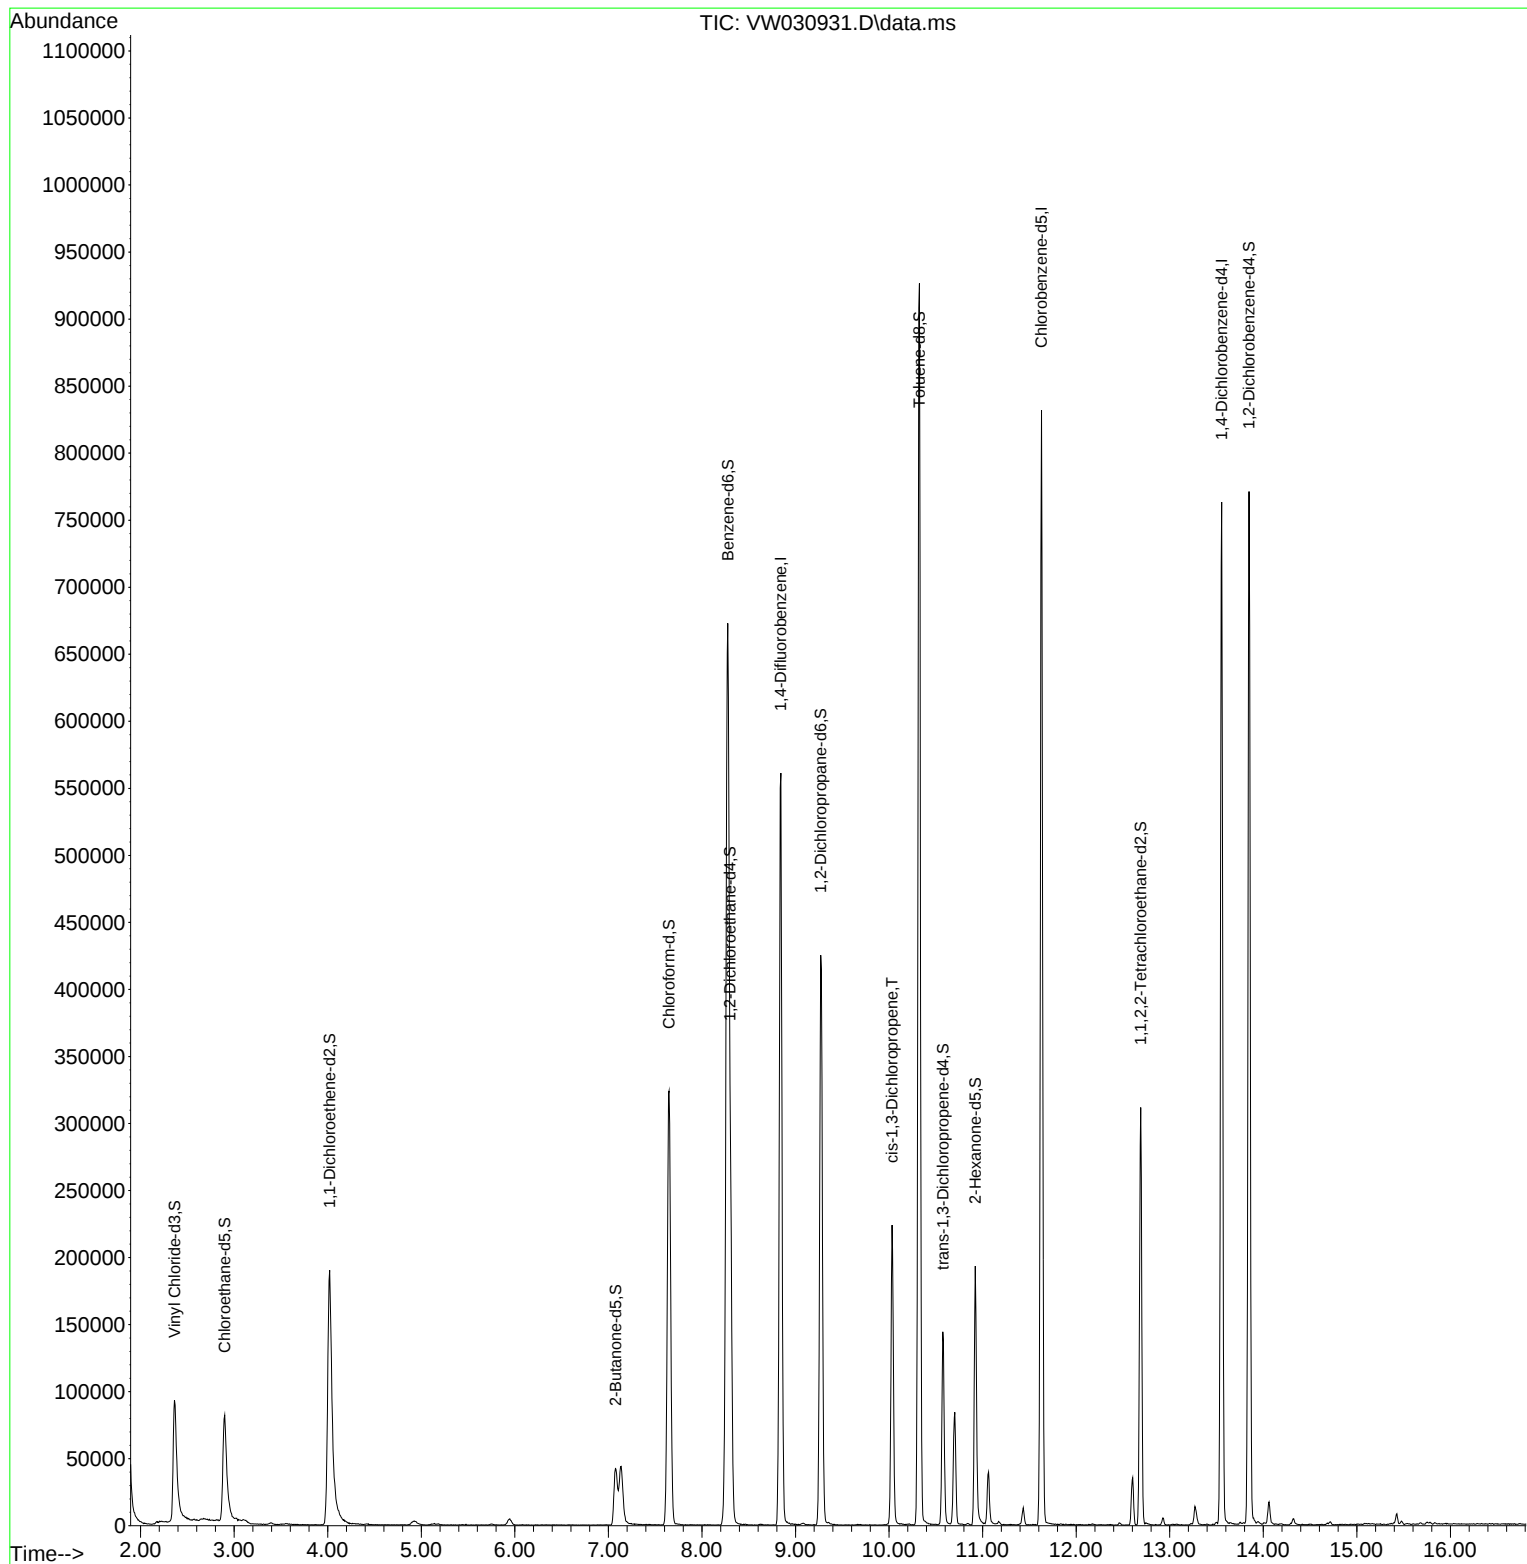

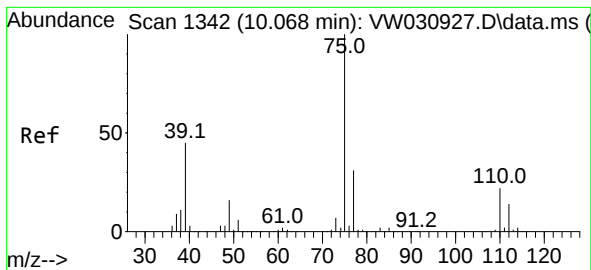

#39
 cis-1,3-Dichloropropene
 Concen: 0.493 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030931.D
 Acq: 05 Nov 2024 12:14

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5441
 Ion Ratio Lower Upper
 75 100
 77 41.4 21.3 39.6#

