
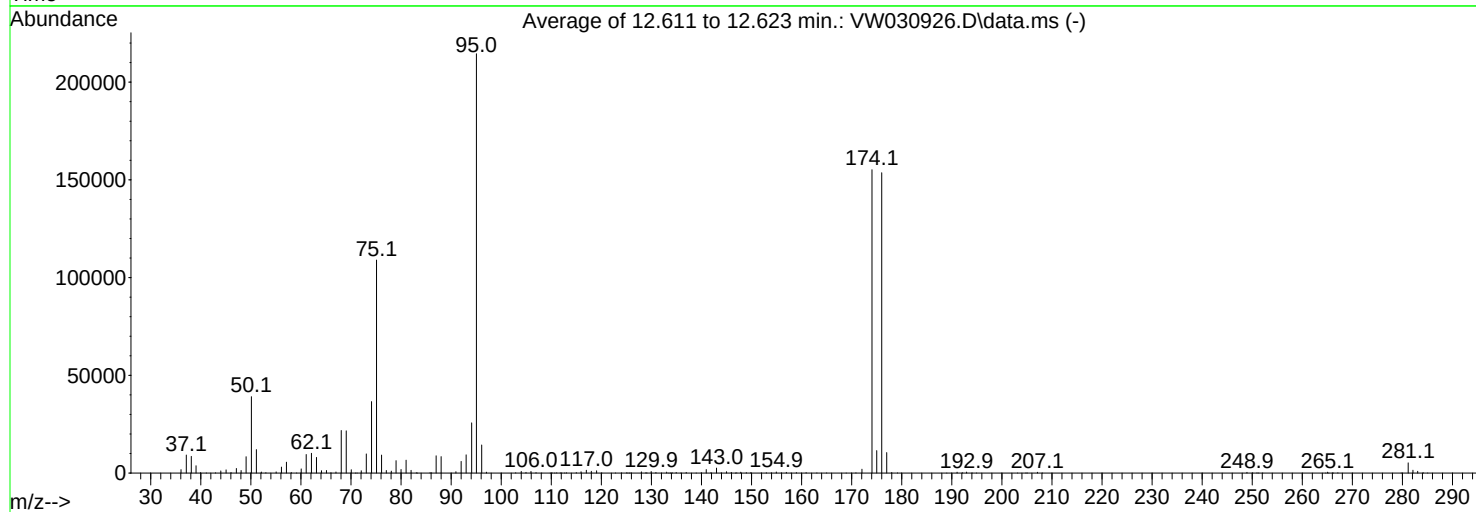


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110524\
Data File : VW030926.D
Acq On : 05 Nov 2024 08:24
Operator : SY/MD
Sample : BFB591
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB591

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Wed Nov 06 00:11:36 2024

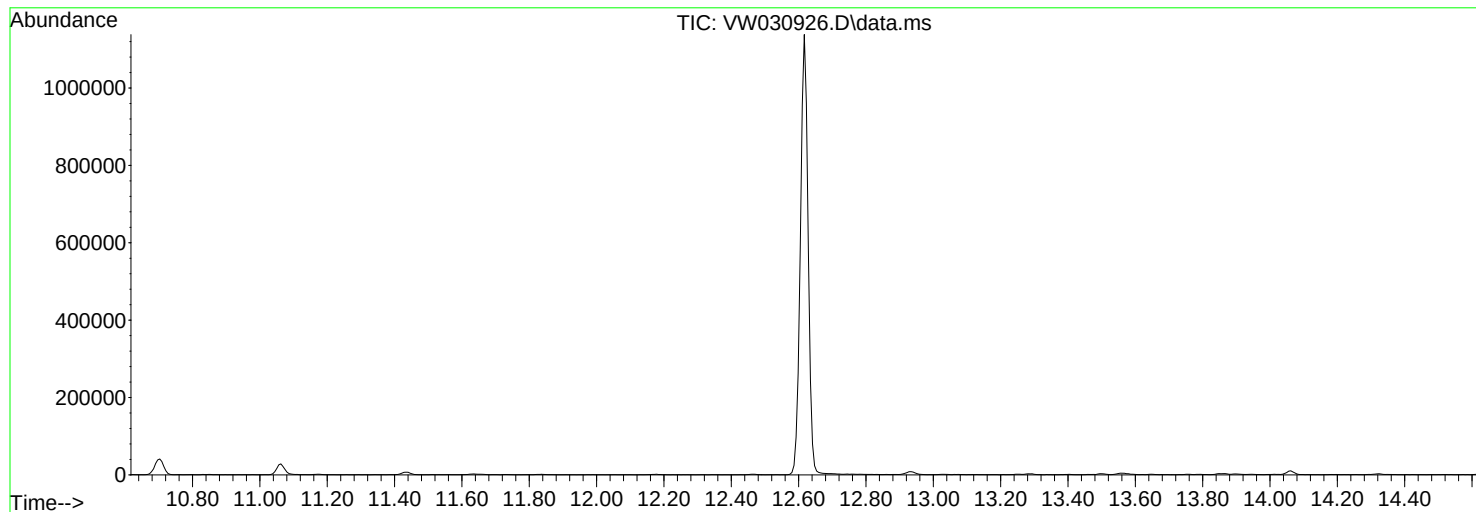

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	39099	PASS
75	95	30	80	50.8	108981	PASS
95	95	100	100	100.0	214528	PASS
96	95	5	9	6.7	14380	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.3	155205	PASS
175	174	5	9	7.4	11502	PASS
176	174	95	101	99.0	153645	PASS
177	176	5	9	6.8	10494	PASS

m/z	Abundance
39.90	207.0
44.00	207.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

m/z	Abundance
36.10	1877.0
37.10	9802.0
38.10	8765.0
39.00	4085.0
40.00	296.0
41.10	96.0
43.00	161.0
44.00	1510.0
45.10	1505.0
46.10	300.0
47.10	2186.0
48.10	1171.0
49.00	8263.0
50.10	39584.0
51.10	12104.0
52.10	483.0
53.00	225.0
55.10	570.0
56.10	3049.0
57.10	5505.0
58.20	178.0
59.20	180.0
60.10	2035.0
61.00	9722.0
62.10	10368.0
63.10	8466.0
64.10	1323.0
65.10	1602.0
66.00	185.0
67.00	654.0
68.10	21808.0
69.00	21440.0
70.00	1640.0
71.20	127.0
72.00	1265.0
73.00	9884.0
74.10	36792.0
75.10	107112.0
76.10	8932.0
77.10	1300.0
78.00	940.0
79.00	6661.0
80.00	1760.0
81.00	6617.0
82.00	1474.0
83.00	239.0
86.10	343.0
87.00	9049.0
88.00	8049.0
91.00	798.0
92.00	5535.0
93.00	8573.0
94.10	25504.0
95.00	200576.0
96.10	14189.0
97.00	297.0
102.90	225.0
104.00	823.0
105.00	314.0
106.00	875.0
107.00	316.0
108.10	55.0
110.10	95.0
111.10	147.0
111.90	162.0
112.70	149.0
113.10	148.0
115.10	274.0
116.00	724.0
117.00	1462.0
118.00	1001.0
119.10	1213.0
123.00	99.0
124.10	70.0
125.10	300.0
125.60	137.0
126.00	137.0
128.00	604.0
128.90	270.0
130.00	852.0
130.90	339.0
132.00	87.0
133.10	733.0
133.80	250.0
134.20	201.0
135.00	348.0
135.90	51.0
137.00	341.0
140.00	115.0
140.90	1712.0
143.00	2559.0
144.00	246.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

145.00	973.0
146.00	351.0
147.00	199.0
147.80	363.0
149.00	260.0
149.90	202.0
151.90	54.0
152.90	77.0
153.90	106.0
155.00	509.0
155.90	139.0
157.00	356.0
157.90	54.0
159.00	183.0
160.90	245.0
163.10	169.0
165.00	189.0
170.90	317.0
172.00	2470.0
174.10	129360.0
175.00	9721.0
176.00	128584.0
177.00	8379.0
177.90	246.0
179.10	198.0
189.00	52.0
191.00	769.0
192.10	270.0
192.90	745.0
194.10	103.0
195.00	71.0
203.20	68.0
204.80	176.0
207.10	609.0
208.10	113.0
249.00	662.0
250.20	157.0
250.90	215.0
251.30	145.0
252.10	58.0
265.10	788.0
266.00	301.0
267.10	240.0
279.70	91.0
281.10	7902.0
282.10	2252.0
283.10	1473.0
284.10	275.0
285.00	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

m/z	Abundance
36.00	1908.0
37.10	10510.0
38.10	10009.0
39.10	4298.0
40.00	390.0
41.10	92.0
42.90	159.0
44.10	1355.0
45.10	1964.0
46.10	228.0
47.10	2807.0
48.00	1676.0
49.10	9619.0
50.10	44184.0
51.10	13117.0
52.10	801.0
53.00	279.0
55.00	745.0
56.10	3511.0
57.10	6346.0
58.00	274.0
59.10	78.0
60.00	2505.0
61.10	10198.0
62.10	11362.0
63.10	9036.0
64.10	1315.0
65.10	1372.0
65.90	194.0
67.00	496.0
68.10	24080.0
69.10	23912.0
70.00	1839.0
72.10	1396.0
73.10	10849.0
74.10	40720.0
75.10	121840.0
76.10	10592.0
77.10	1435.0
78.10	1060.0
79.00	6802.0
80.00	1946.0
81.00	7381.0
82.00	1542.0
83.10	188.0
85.80	275.0
87.00	9888.0
88.00	10115.0
91.00	789.0
92.00	6928.0
93.00	10816.0
94.10	29128.0
95.10	242816.0
96.10	16381.0
97.00	484.0
102.90	143.0
104.00	950.0
104.90	379.0
106.00	1070.0
106.90	273.0
109.80	109.0
110.20	100.0
111.10	245.0
111.70	160.0
112.20	104.0
113.00	190.0
115.00	264.0
115.90	779.0
117.00	1683.0
118.00	948.0
119.00	1424.0
120.10	84.0
122.80	98.0
124.10	173.0
125.30	258.0
125.80	132.0
128.00	710.0
128.90	348.0
130.00	915.0
130.90	384.0
133.00	498.0
134.10	172.0
134.90	325.0
135.90	89.0
136.90	352.0
139.00	106.0
139.90	158.0
141.00	2063.0
141.90	374.0
143.00	2806.0
144.00	127.0
145.00	709.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

146.00	286.0
147.10	215.0
147.90	469.0
148.90	298.0
149.80	212.0
152.00	123.0
153.00	203.0
153.80	91.0
155.00	673.0
156.00	148.0
156.90	425.0
158.80	297.0
160.90	304.0
163.10	103.0
165.00	124.0
168.90	69.0
172.10	1990.0
174.00	164928.0
175.00	13323.0
176.00	176704.0
177.00	11256.0
178.00	288.0
179.20	103.0
191.10	410.0
192.20	191.0
193.00	552.0
194.00	151.0
194.90	82.0
203.10	53.0
205.10	143.0
207.10	408.0
248.90	372.0
250.00	135.0
251.00	153.0
265.00	613.0
266.20	113.0
267.10	154.0
279.80	51.0
281.20	5347.0
282.10	1475.0
283.00	921.0
284.20	249.0
285.10	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

m/z	Abundance
36.00	1499.0
37.10	7387.0
38.10	6846.0
39.10	2888.0
40.00	343.0
41.00	54.0
43.00	165.0
44.00	1053.0
45.00	1488.0
45.90	191.0
47.10	2086.0
48.10	1121.0
49.10	7226.0
50.10	33528.0
51.10	10834.0
52.10	359.0
53.00	166.0
55.10	519.0
56.10	2663.0
57.10	4853.0
58.10	199.0
60.00	1843.0
61.10	8608.0
62.10	8609.0
63.10	6514.0
64.10	1035.0
65.10	1017.0
66.10	93.0
67.00	550.0
68.00	19480.0
69.10	19496.0
70.10	1698.0
70.90	63.0
72.00	1008.0
73.10	8647.0
74.10	32224.0
75.10	97992.0
76.10	8137.0
77.00	1257.0
78.00	1025.0
79.00	5627.0
80.00	1816.0
81.00	5801.0
82.00	1207.0
83.00	94.0
83.30	92.0
85.80	307.0
87.00	7621.0
88.00	7101.0
90.90	585.0
92.00	5462.0
93.00	8596.0
94.10	22448.0
95.10	200192.0
96.10	12569.0
97.10	598.0
102.90	136.0
104.00	817.0
105.00	389.0
105.90	680.0
107.00	151.0
110.10	157.0
110.70	70.0
111.10	99.0
112.00	138.0
113.00	113.0
114.90	216.0
116.00	590.0
117.00	1210.0
118.00	786.0
119.00	919.0
120.10	52.0
122.70	64.0
124.00	86.0
125.00	120.0
126.00	161.0
128.00	629.0
129.10	350.0
129.90	634.0
130.90	261.0
132.90	221.0
133.50	113.0
134.10	82.0
134.90	318.0
137.00	330.0
138.90	52.0
140.00	109.0
141.00	1710.0
141.90	340.0
143.00	2281.0
143.90	169.0
144.90	488.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591

145.90	391.0
146.80	148.0
147.90	535.0
148.90	129.0
149.80	221.0
152.00	111.0
153.00	227.0
154.00	239.0
154.90	526.0
156.00	103.0
157.00	351.0
159.00	258.0
160.90	212.0
162.90	54.0
168.90	50.0
170.70	93.0
172.10	1502.0
174.00	171328.0
175.00	11463.0
176.00	155648.0
177.00	11846.0
178.10	290.0
190.90	218.0
192.10	105.0
193.00	306.0
205.00	59.0
207.10	237.0
249.10	165.0
264.70	75.0
265.30	116.0
267.00	97.0
281.00	2474.0
282.20	696.0
283.20	386.0

Instrument :
MSVOA_W
ClientSampleId :
BFB591