

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110618\
 Data File : VW006700.D
 Acq On : 06 Nov 2018 21:17
 Operator : SY/AP
 Sample : J5815-01
 Misc : 5.53G/5ML/MSVOA W/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 HL-R37719-RT

Quant Time: Nov 07 12:03:24 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 01 03:48:08 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	197851	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	258962	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	151716	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	33366	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	85671	50.37	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.74%	
35) Dibromofluoromethane	7.89	113	92352	56.83	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.66%	
50) Toluene-d8	10.33	98	225516	36.45	ug/l	0.00
Spiked Amount 50.000			Recovery	=	72.90%	
62) 4-Bromofluorobenzene	12.62	95	45284	20.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	40.38%	
Target Compounds						
16) Acetone	4.14	43	2873	10.463	ug/l #	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110618\
Data File : VW006700.D
Acq On : 06 Nov 2018 21:17
Operator : SY/AP
Sample : J5815-01
Misc : 5.53G/5ML/MSVOA W/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
HL-R37719-RT

Quant Time: Nov 07 12:03:24 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 01 03:48:08 2018
Response via : Initial Calibration

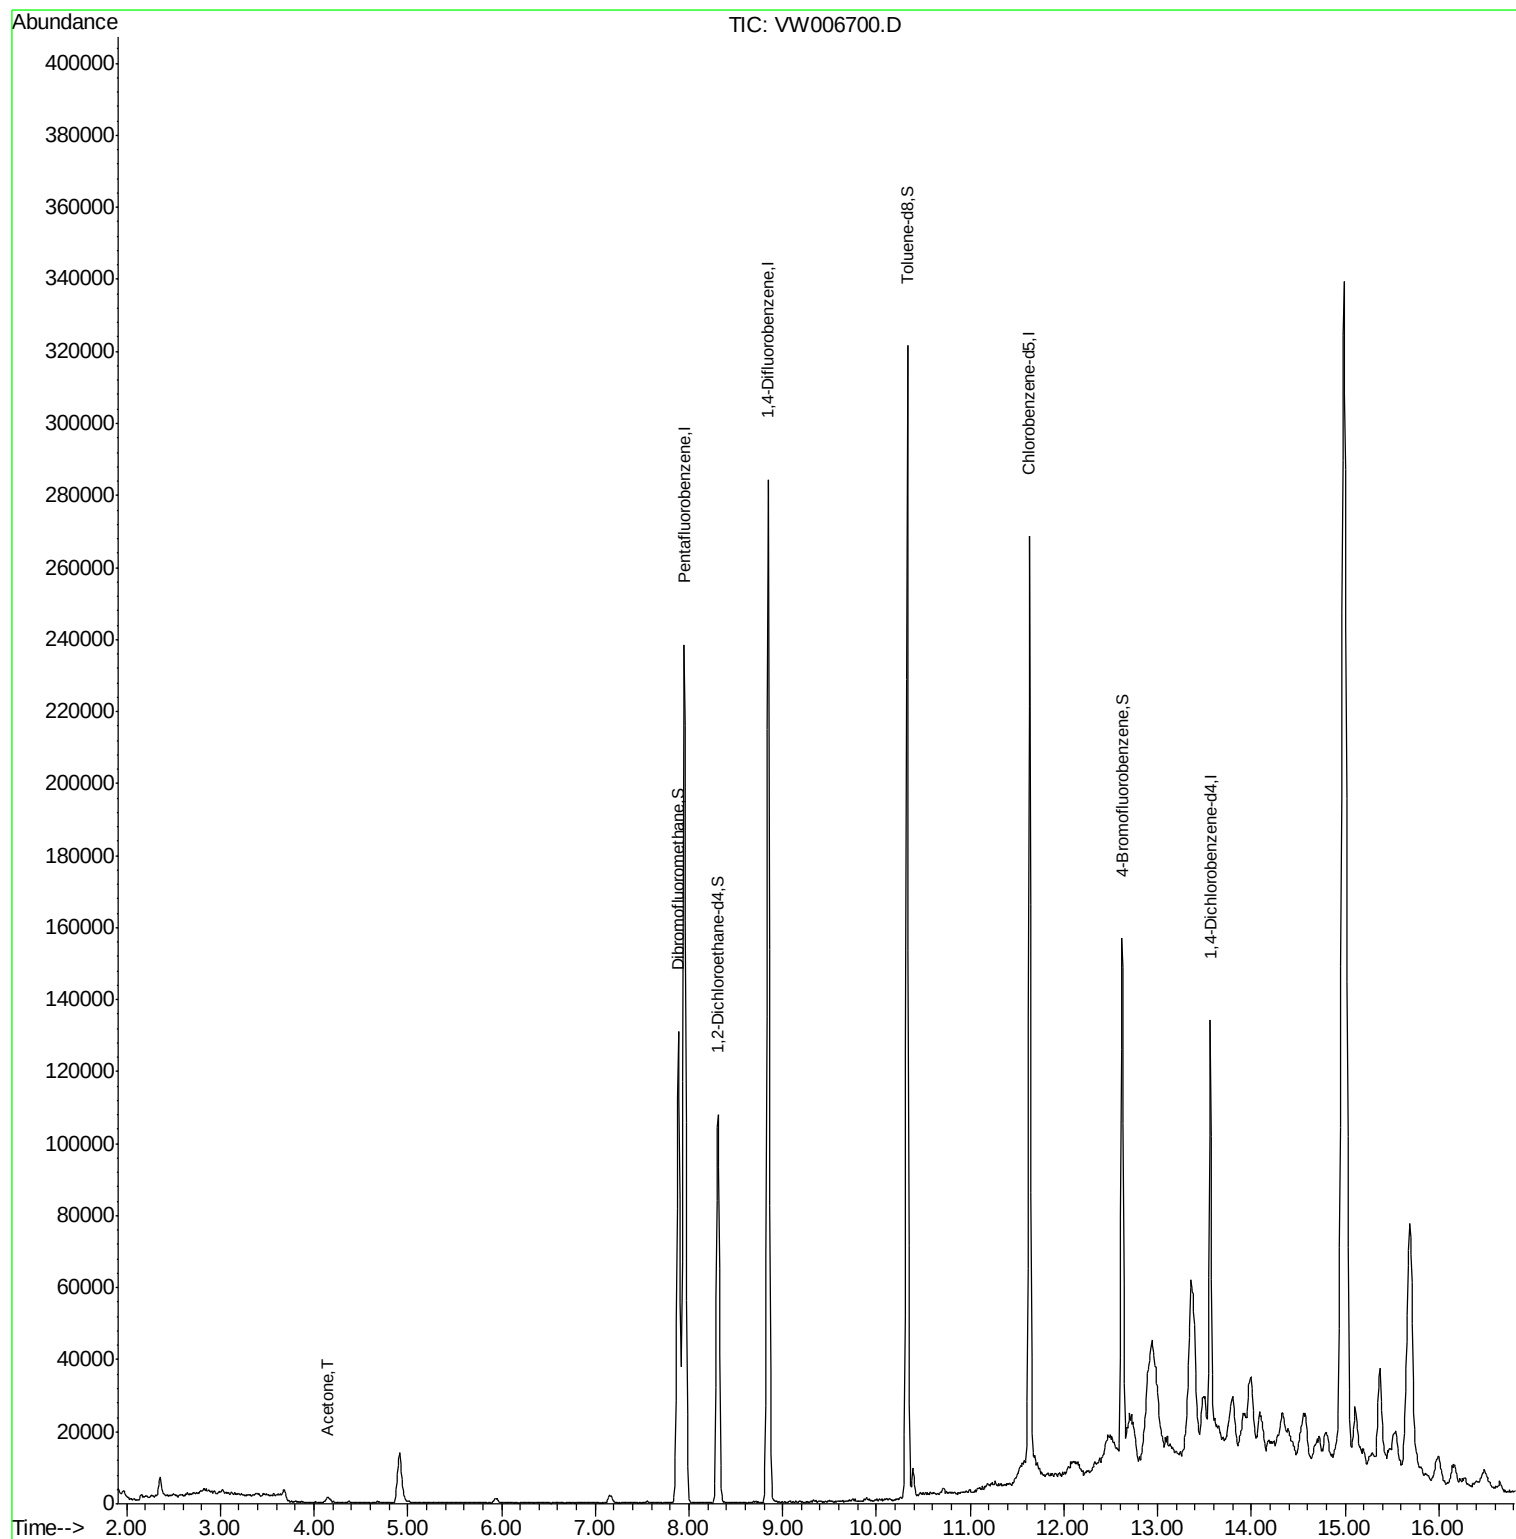

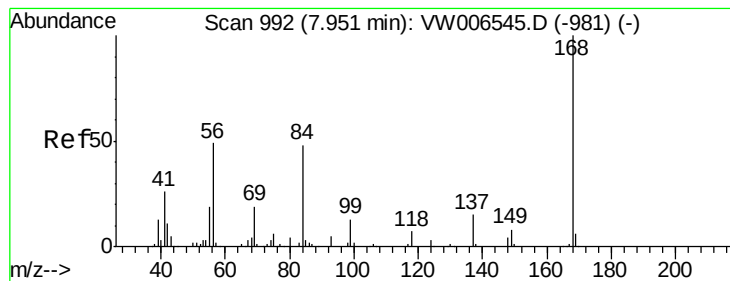

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.00 min

Lab File: VW006700.D

Acq: 06 Nov 2018 21:17

Instrument :

MSVOA_W

ClientSampleId :


HL-R37719-RT

Tot Ion:168 Resp: 197851

Ion Ratio Lower Upper




168 100

99 47.6 37.4 56.0

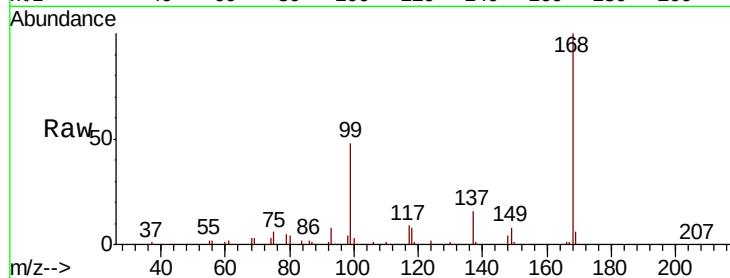

Abundance Ion 167.90 (167.60 to 168.60): VW

Ion 98.90 (98.60 to 99.60): VW

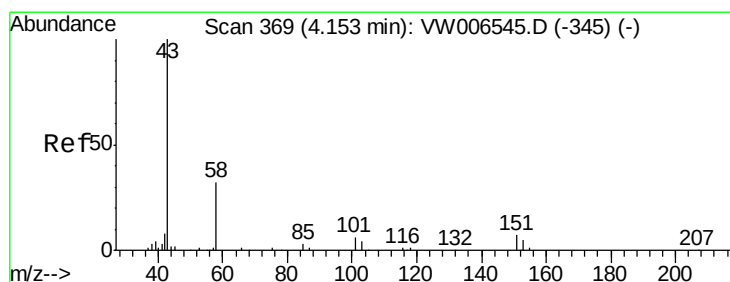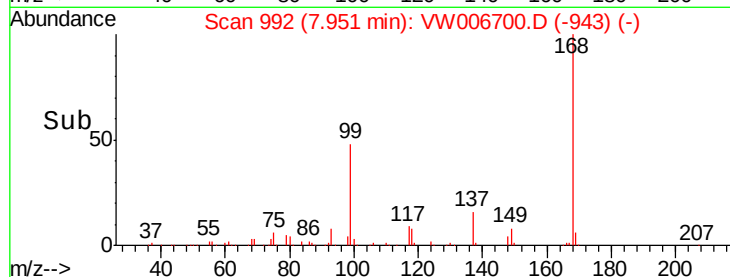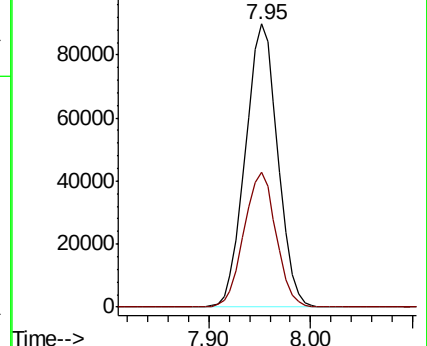

#16

Acetone

Concen: 10.463 ug/l

RT: 4.14 min Scan# 367

Delta R.T. -0.01 min

Lab File: VW006700.D


Acq: 06 Nov 2018 21:17

Tgt Ion: 43 Resp: 2873

Ion Ratio Lower Upper



43 100


58 25.2 25.8 38.8#

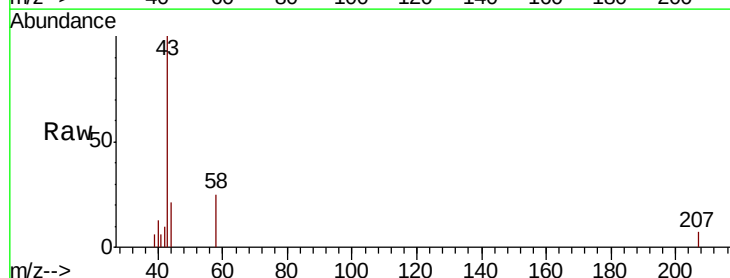

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



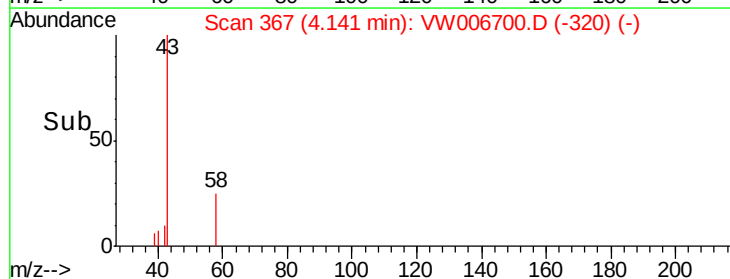
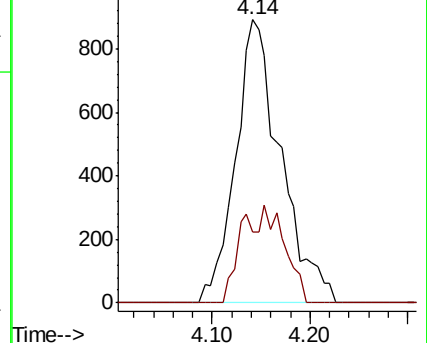


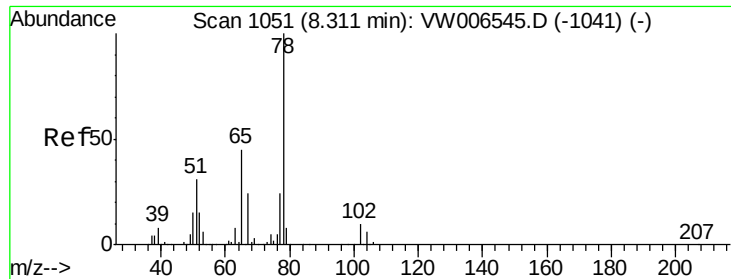

#33
 1,2-Dichloroethane-d4
 Concen: 50.373 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: VW006700.D
 Acq: 06 Nov 2018 21:17




Instrument :
 MSVOA_W
 ClientSampleId :
 HL-R37719-RT


Tot Ion: 65 Resp: 85671
 Ion Ratio Lower Upper
 65 100
 67 52.5 0.0 104.4

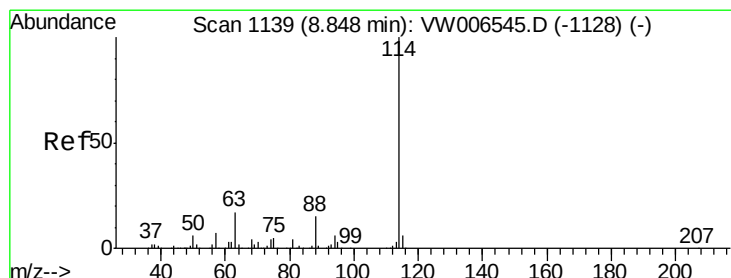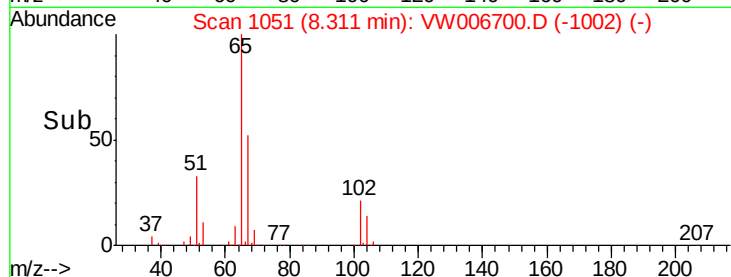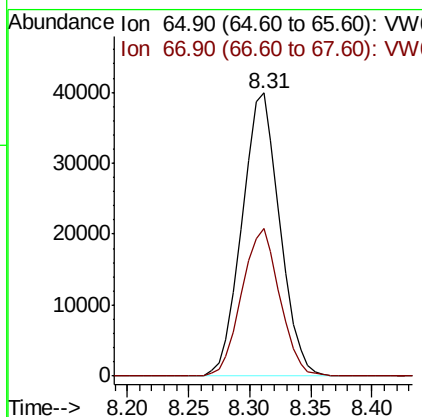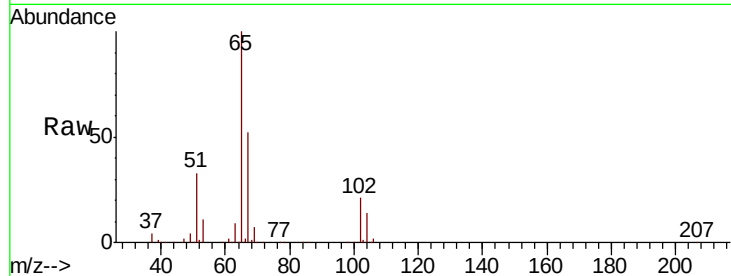

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. -0.00 min
 Lab File: VW006700.D
 Acq: 06 Nov 2018 21:17

Tgt Ion: 114 Resp: 258962
 Ion Ratio Lower Upper
 114 100
 63 16.9 0.0 34.4
 88 14.4 0.0 29.0


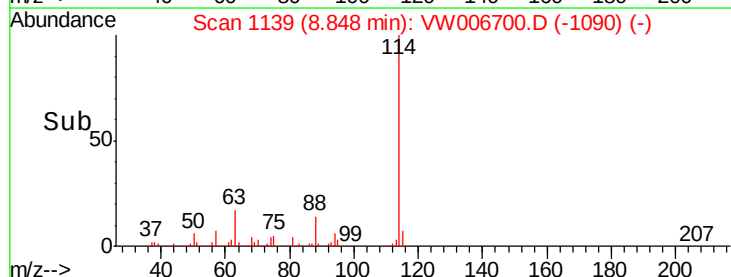
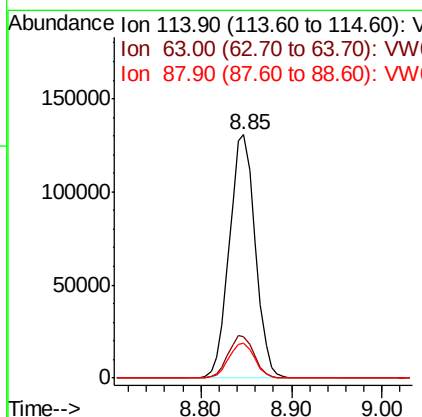
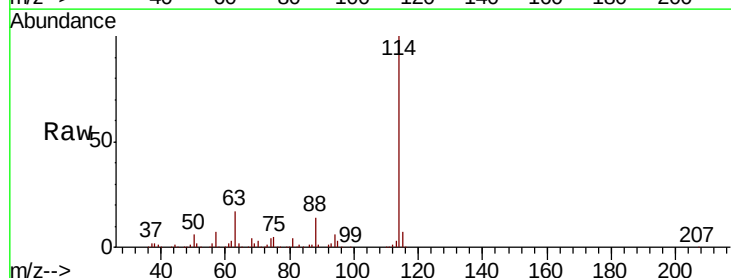


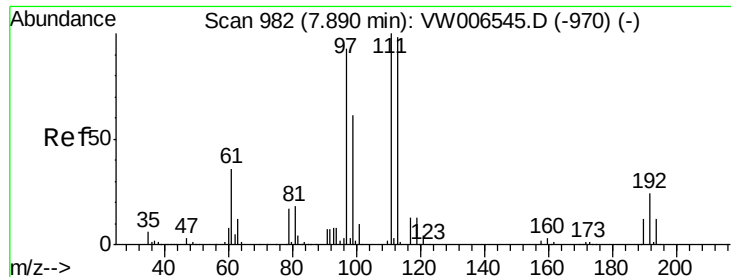

#35
 Dibromofluoromethane
 Concen: 56.825 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. -0.00 min
 Lab File: VW006700.D
 Acq: 06 Nov 2018 21:17




Instrument :
 MSVOA_W
 ClientSampleId :
 HL-R37719-RT


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.8	82.2	123.2
192	23.7	19.0	28.6

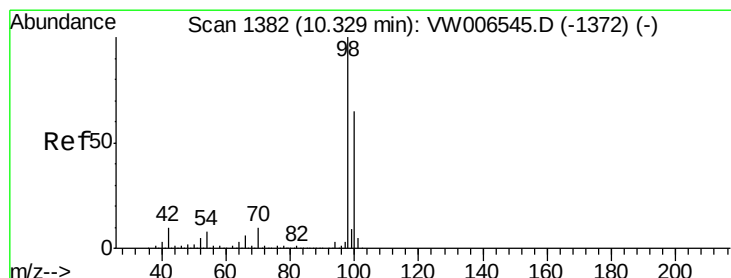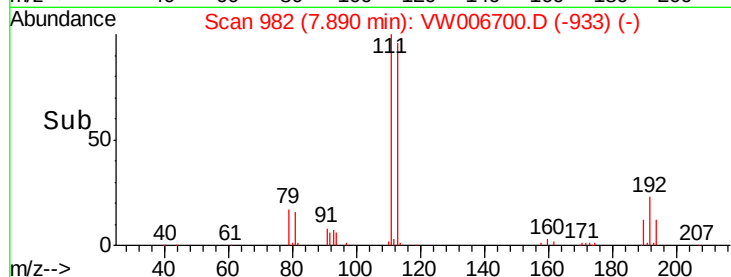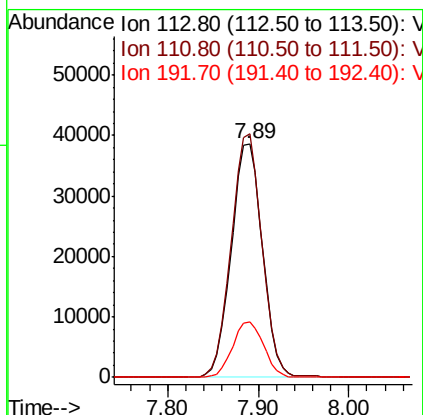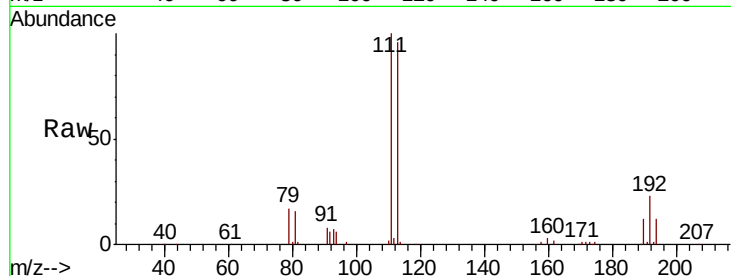

#50
 Toluene-d8
 Concen: 36.451 ug/l
 RT: 10.33 min Scan# 1382
 Delta R.T. -0.00 min
 Lab File: VW006700.D
 Acq: 06 Nov 2018 21:17

Tgt Ion	Ratio	Lower	Upper
98	100		
100	63.5	51.6	77.4

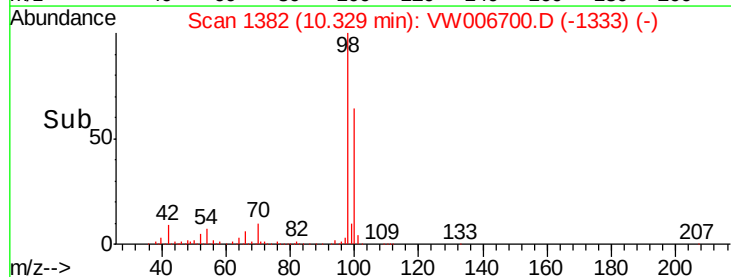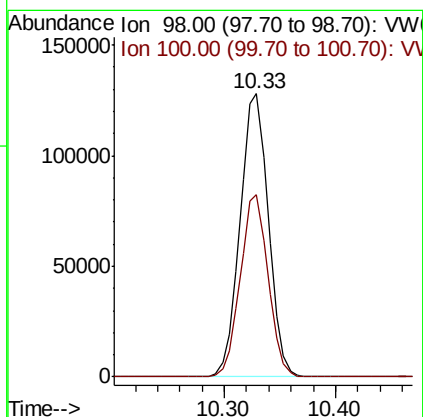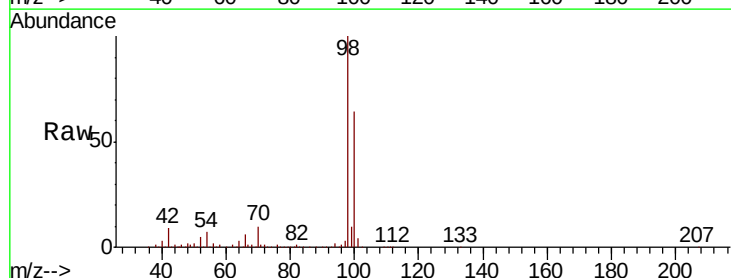

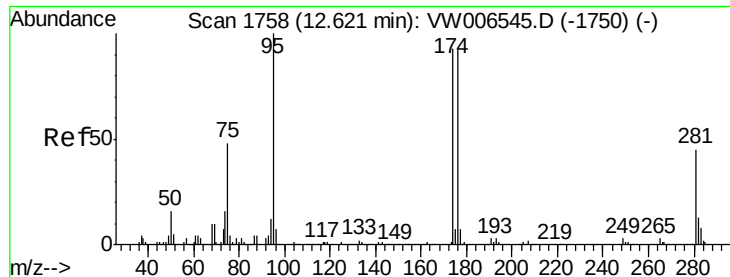

#62

4-Bromofluorobenzene

Concen: 20.189 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW006700.D

Acq: 06 Nov 2018 21:17

Instrument :

MSVOA_W

ClientSampleId :

HL-R37719-RT


Tot Ion: 95 Resp: 45284

Ion Ratio Lower Upper

95 100

174 94.8 0.0 192.4




176 93.8 0.0 187.4

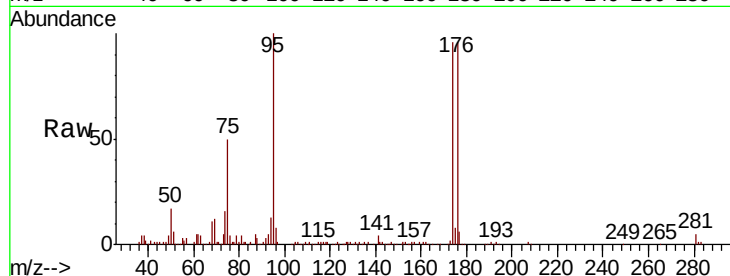

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

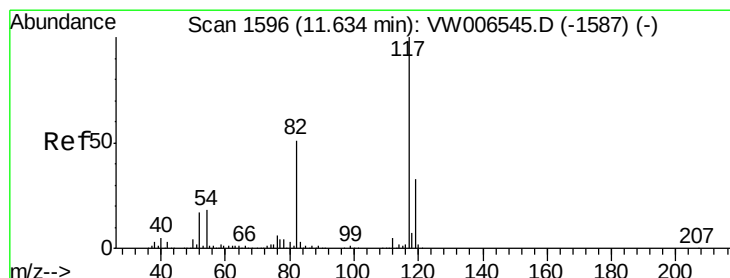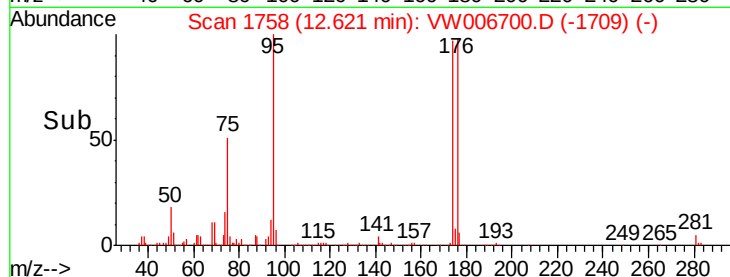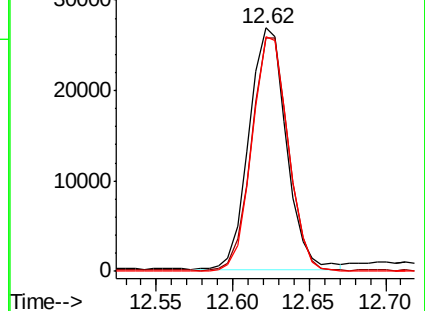

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. -0.00 min

Lab File: VW006700.D

Acq: 06 Nov 2018 21:17


Tgt Ion: 117 Resp: 151716

Ion Ratio Lower Upper

117 100

82 49.6 40.8 61.2



119 31.3 26.1 39.1

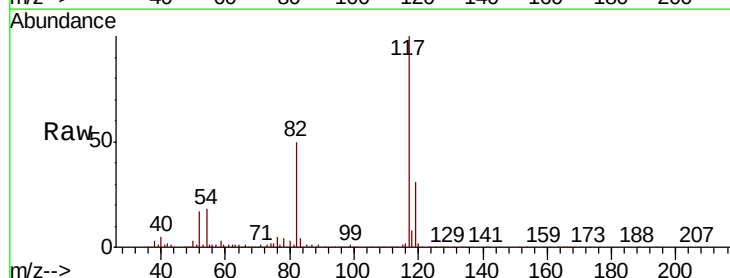


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

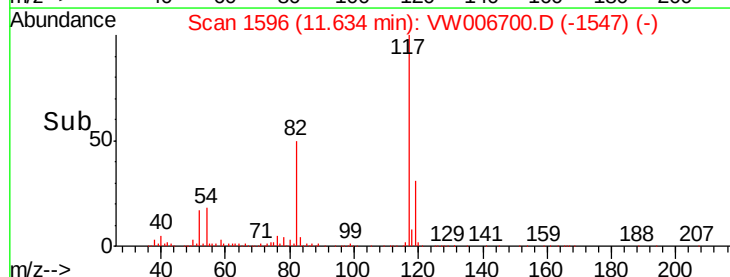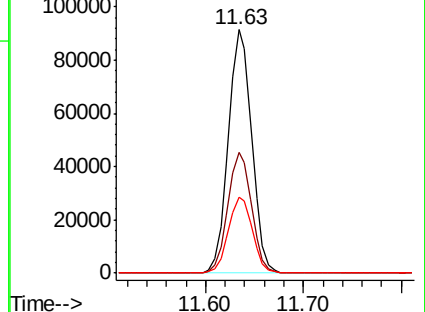


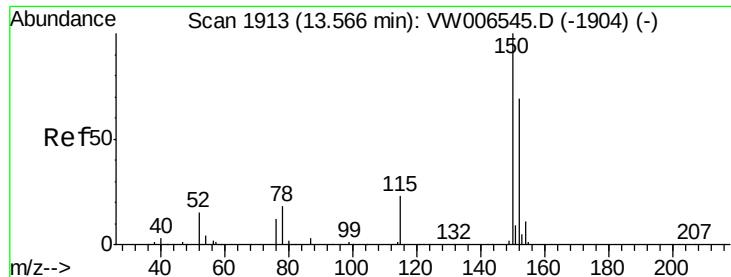

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.57 min Scan# 1913
 Delta R.T. -0.00 min
 Lab File: VW006700.D
 Acq: 06 Nov 2018 21:17

Instrument :
 MSVOA_W
 ClientSampleId :
 HL-R37719-RT

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.9	26.6	79.8
150	156.4	0.0	344.6

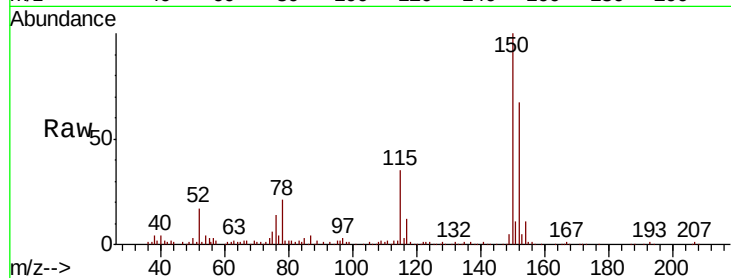

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

