


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110618\
Data File : VW006705.D
Acq On : 07 Nov 2018 00:18
Operator : SY/AP
Sample : BFB
Misc : 5.07G/5ML/MSVOA W/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Title : SW846 8260
Last Update : Thu Nov 01 03:48:08 2018

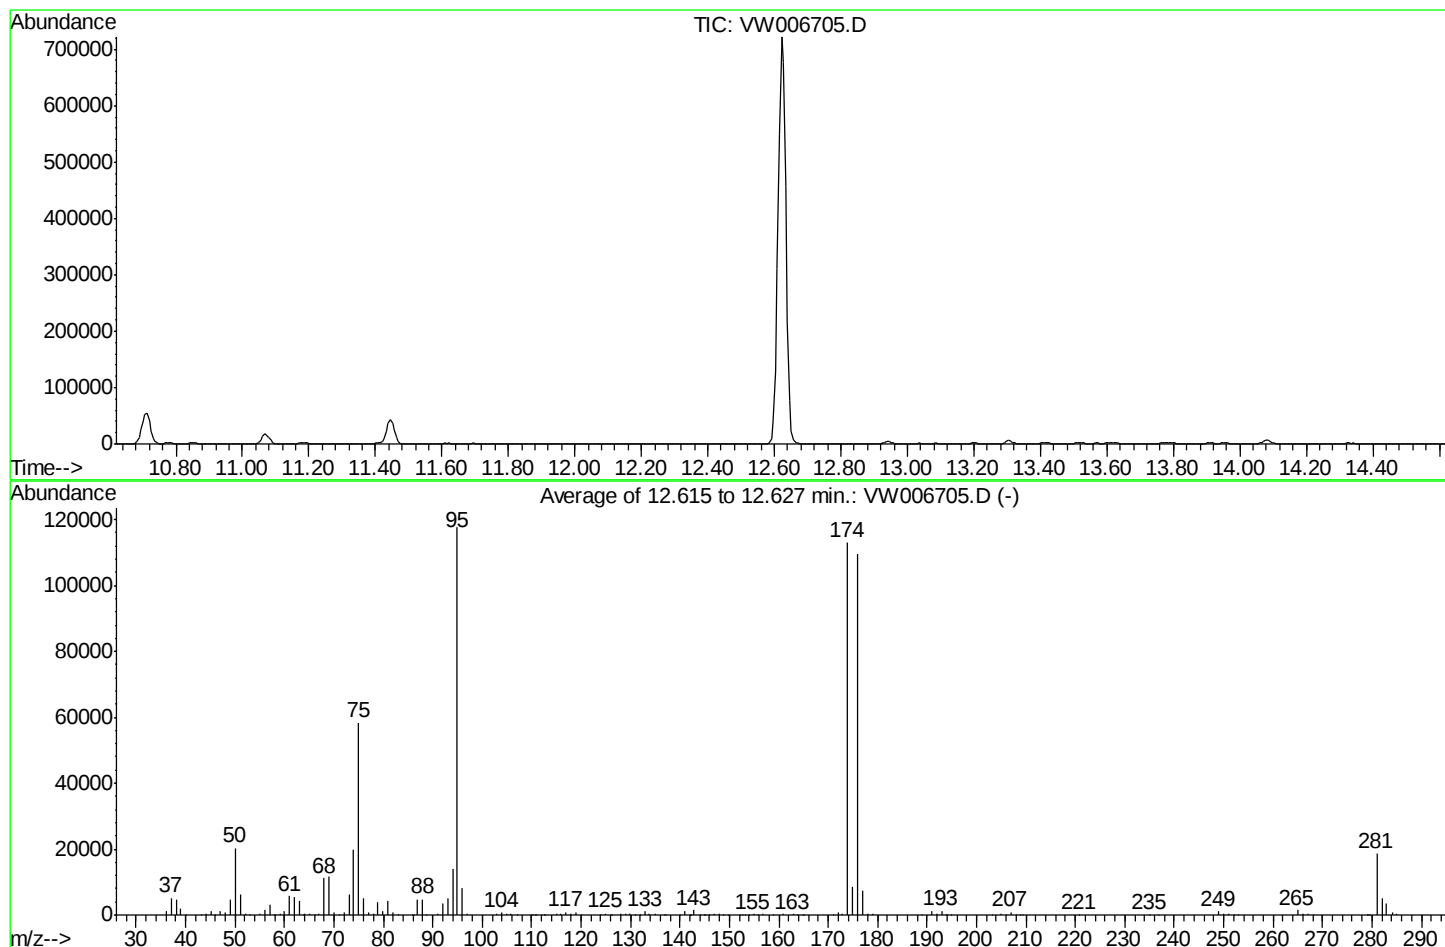

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	20248	PASS
75	95	30	60	49.5	58290	PASS
95	95	100	100	100.0	117672	PASS
96	95	5	9	6.8	8024	PASS
173	174	0.00	2	0.3	292	PASS
174	95	50	100	96.0	112994	PASS
175	174	5	9	7.5	8486	PASS
176	174	95	101	96.9	109472	PASS
177	176	5	9	6.8	7472	PASS