

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
 Data File : VW030941.D
 Acq On : 06 Nov 2024 11:25
 Operator : SY/MD
 Sample : P4622-15
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 07 03:59:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 07 03:58:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	441830	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	410651	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	179769	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	147961	20.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.680%
7) Chloroethane-d5	2.899	69	115935	20.860	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.440%
11) 1,1-Dichloroethene-d2	4.021	65	64210	21.474	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.880%
21) 2-Butanone-d5	7.075	46	56917	47.729	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.460%
24) Chloroform-d	7.648	84	304566	23.383	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.520%
26) 1,2-Dichloroethane-d4	8.307	65	154267	23.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.280%
32) Benzene-d6	8.270	84	600995	23.558	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.240%
36) 1,2-Dichloropropane-d6	9.276	67	177586	23.613	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.440%
41) Toluene-d8	10.325	98	527623	23.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.240%
43) trans-1,3-Dichloroprop...	10.575	79	67713	22.212	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.840%
47) 2-Hexanone-d5	10.922	63	47301	48.530	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.060%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	129000	24.620	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	175209	26.756	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4878	0.493	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
Data File : VW030941.D
Acq On : 06 Nov 2024 11:25
Operator : SY/MD
Sample : P4622-15
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 07 03:59:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 07 03:58:00 2024
Response via : Initial Calibration

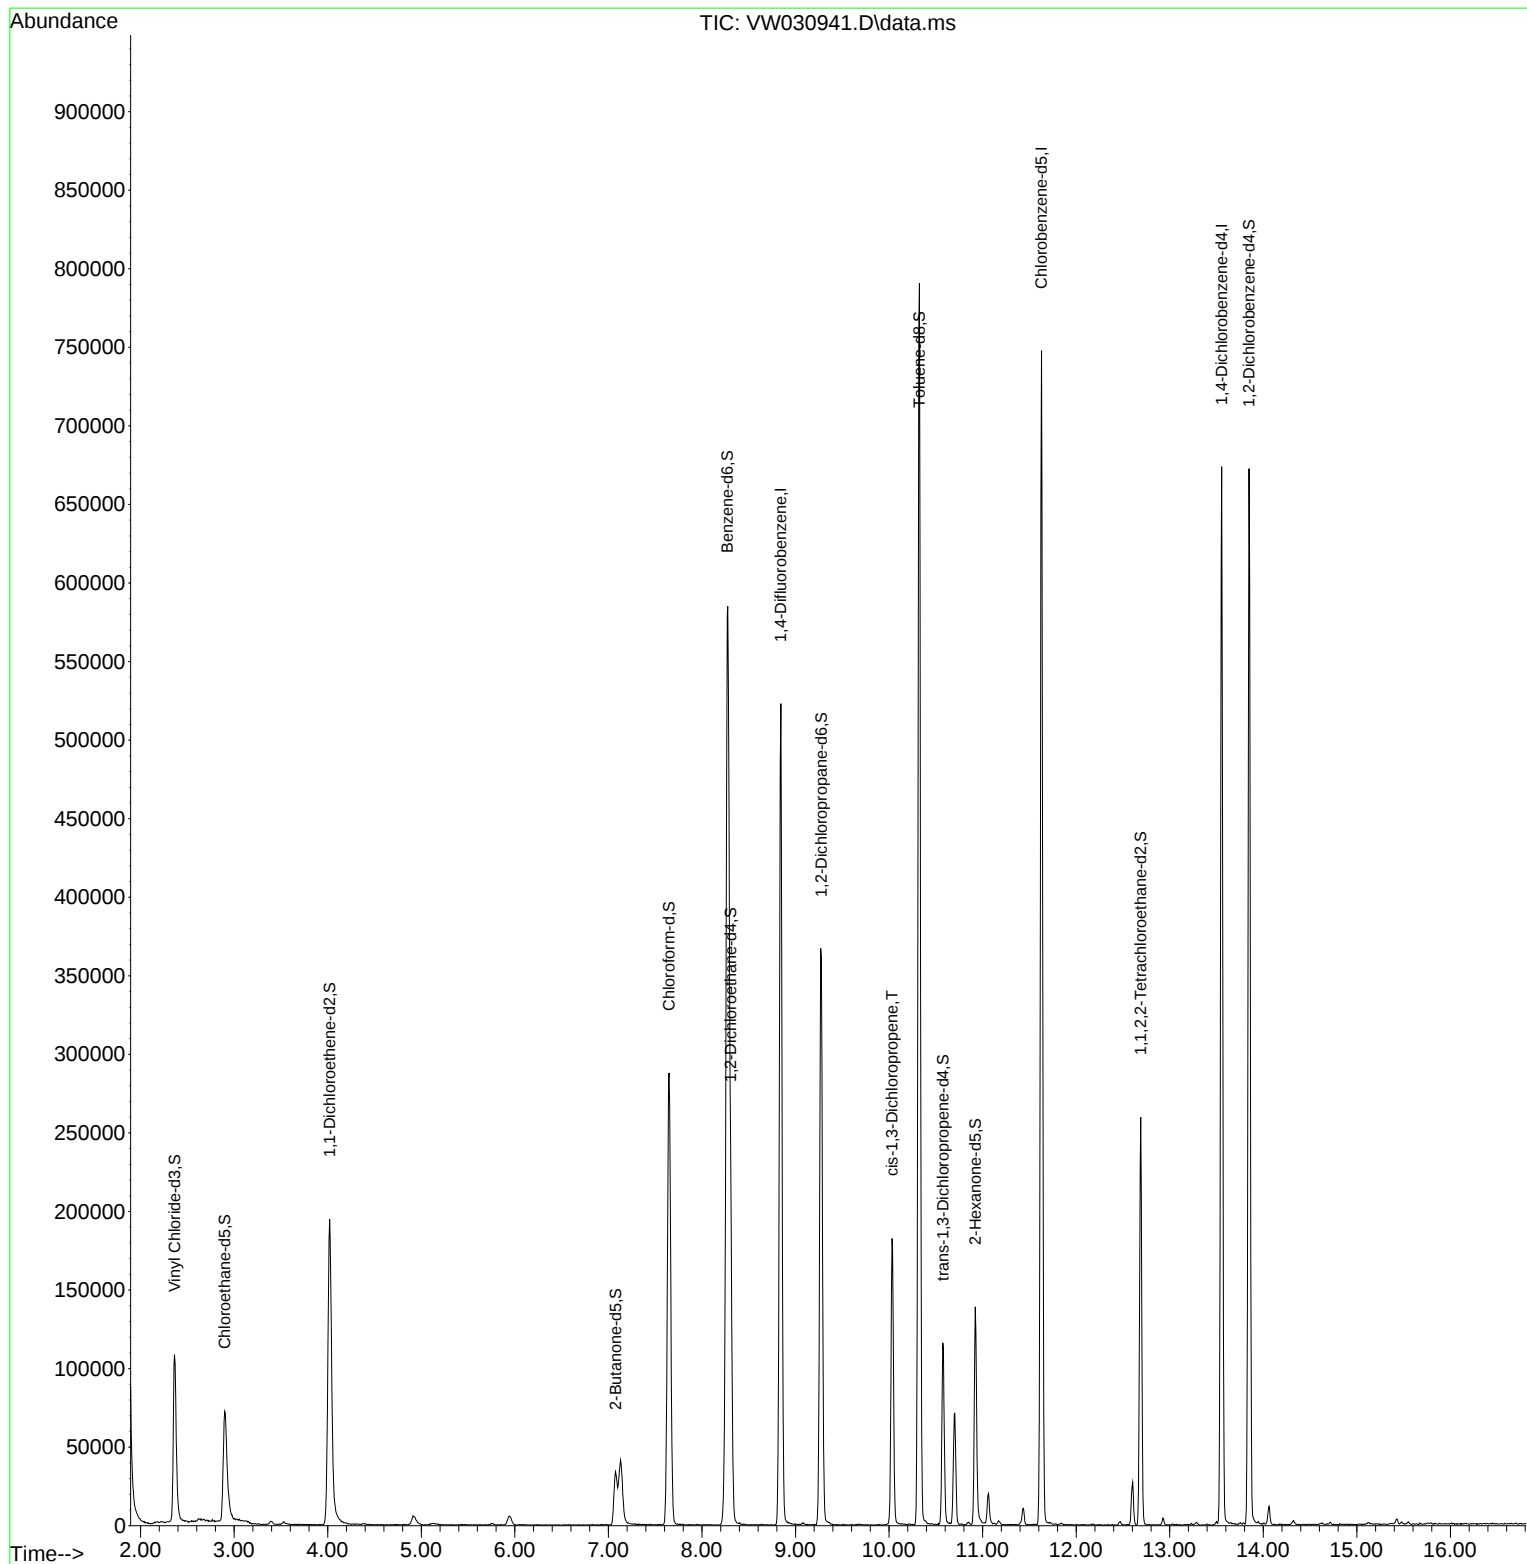

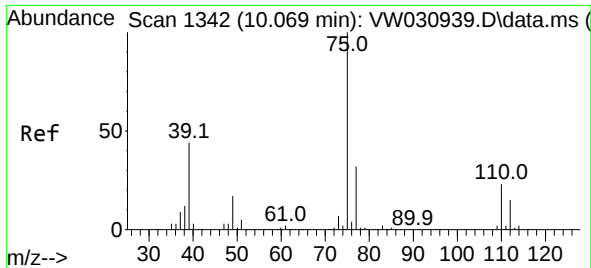

#39
 cis-1,3-Dichloropropene
 Concen: 0.493 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030941.D
 Acq: 06 Nov 2024 11:25

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4878
 Ion Ratio Lower Upper
 75 100
 77 52.0 21.3 39.6#

