

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
 Data File : VW030943.D
 Acq On : 06 Nov 2024 16:06
 Operator : SY/MD
 Sample : P4724-05
 Misc : 5.59g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 07 03:59:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 07 03:58:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	658364	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	593414	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	258694	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	208135	19.276	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.120%
7) Chloroethane-d5	2.905	69	152765	18.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.800%
11) 1,1-Dichloroethene-d2	4.027	65	89026	19.981	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.920%
21) 2-Butanone-d5	7.075	46	100852	56.756	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.520%
24) Chloroform-d	7.654	84	391008	20.146	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.600%
26) 1,2-Dichloroethane-d4	8.307	65	208636	21.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.480%
32) Benzene-d6	8.276	84	776915	21.074	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.280%
36) 1,2-Dichloropropane-d6	9.270	67	234386	21.567	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.280%
41) Toluene-d8	10.325	98	706931	21.379	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.520%
43) trans-1,3-Dichloroprop...	10.575	79	93658	21.261	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.040%
47) 2-Hexanone-d5	10.922	63	79961	56.772	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.540%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	193311	25.531	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	224419	23.816	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	6265	0.438	ug/L	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
Data File : VW030943.D
Acq On : 06 Nov 2024 16:06
Operator : SY/MD
Sample : P4724-05
Misc : 5.59g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 07 03:59:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 07 03:58:00 2024
Response via : Initial Calibration

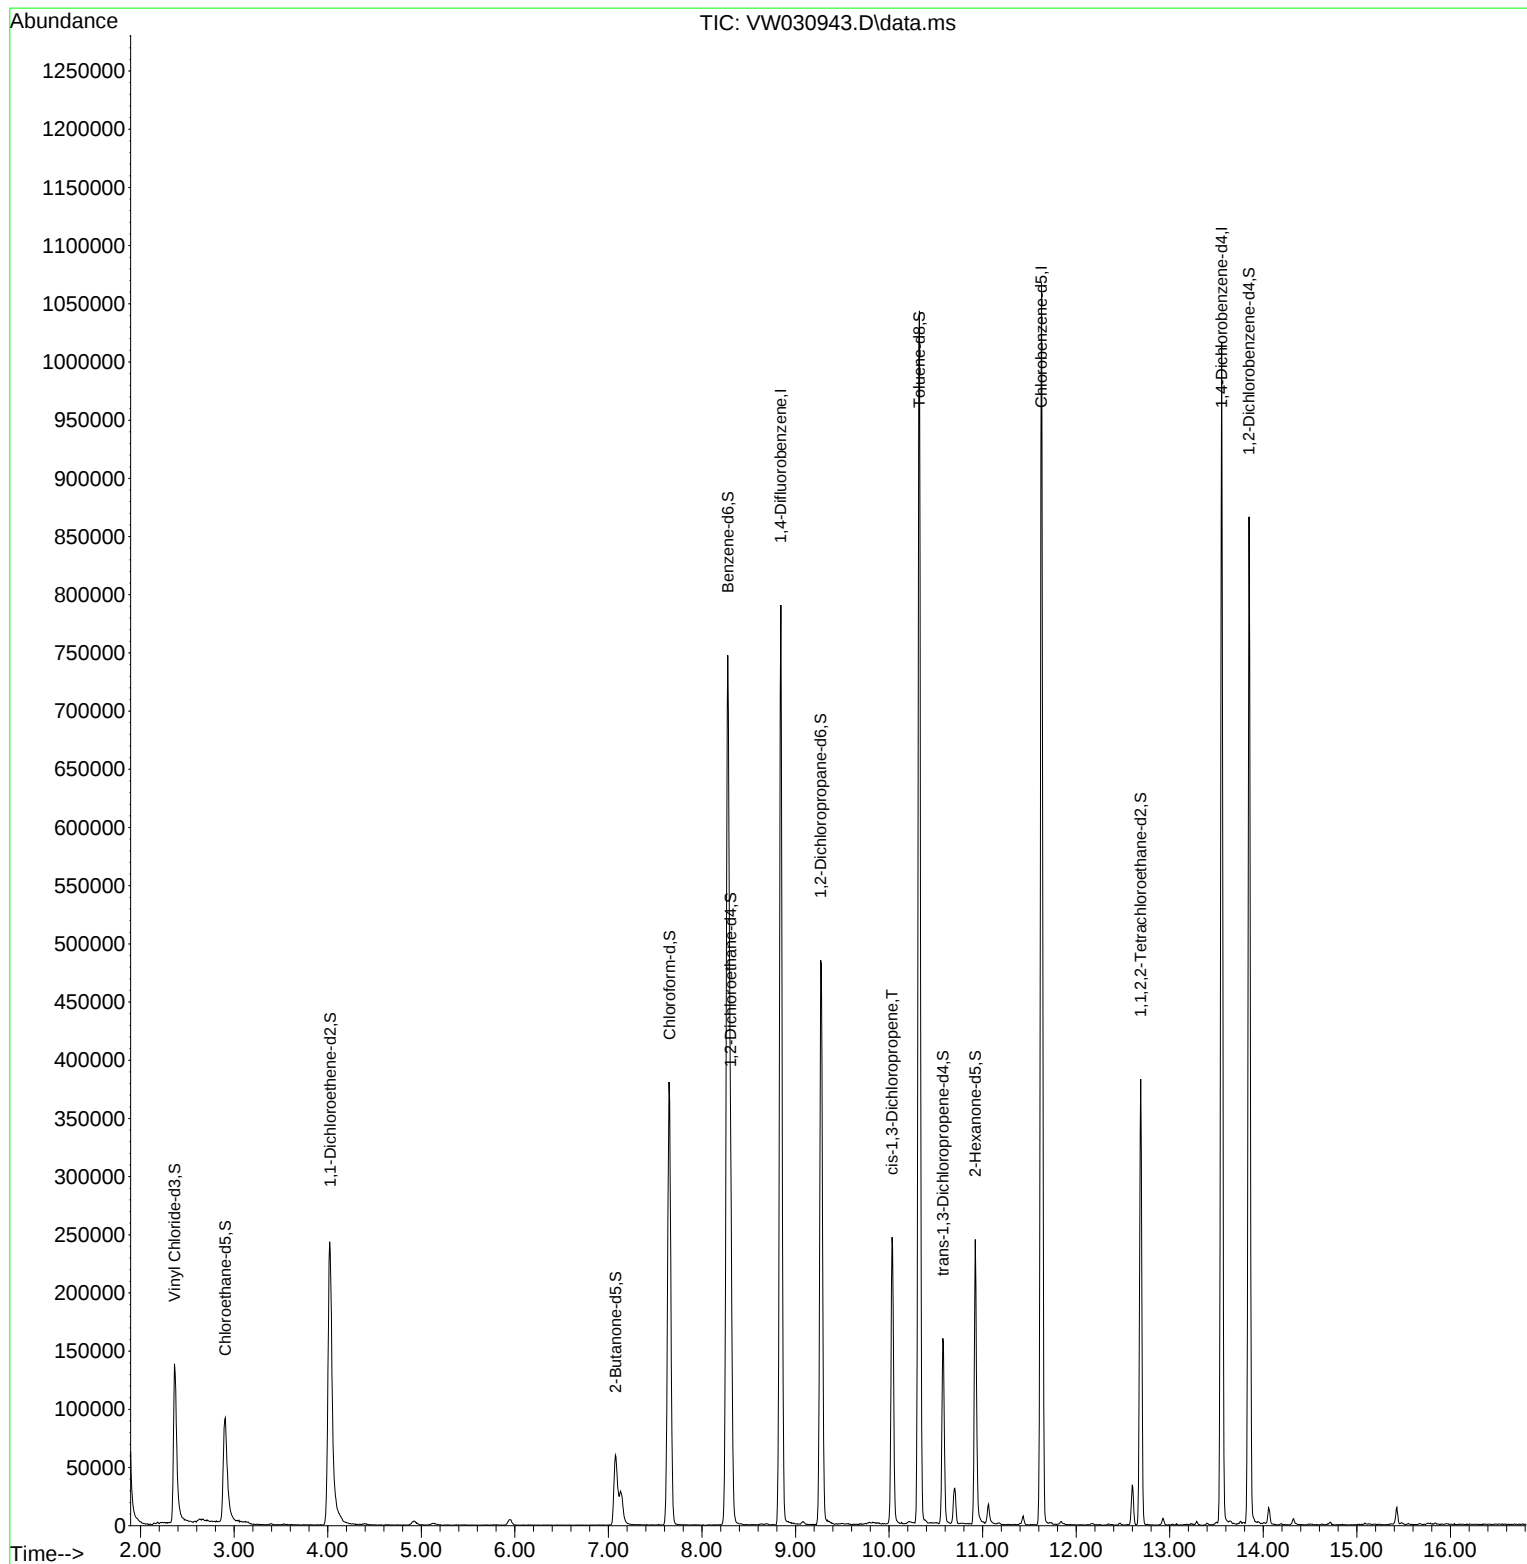

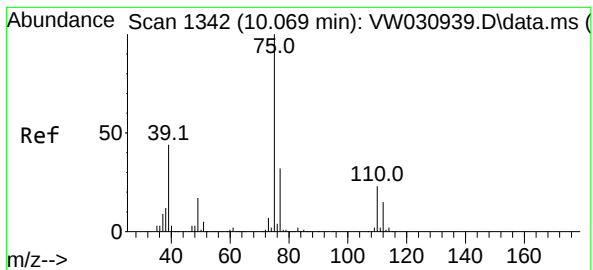

#39
 cis-1,3-Dichloropropene
 Concen: 0.438 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030943.D
 Acq: 06 Nov 2024 16:06

Instrument :
 MSVOA_W
 ClientSampleId :

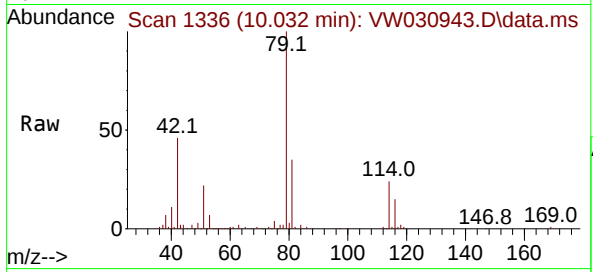

Tgt Ion: 75 Resp: 6265
 Ion Ratio Lower Upper
 75 100
 77 53.2 21.3 39.6#

