

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
 Data File : VW030946.D
 Acq On : 06 Nov 2024 17:18
 Operator : SY/MD
 Sample : P4724-08
 Misc : 5.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 07 03:59:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 07 03:58:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	543956	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	497110	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	194109	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	169632	19.014	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.040%
7) Chloroethane-d5	2.899	69	125565	18.351	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.400%
11) 1,1-Dichloroethene-d2	4.027	65	71900	19.532	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.120%
21) 2-Butanone-d5	7.075	46	89350	60.859	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.720%
24) Chloroform-d	7.648	84	325150	20.276	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.120%
26) 1,2-Dichloroethane-d4	8.307	65	178771	22.422	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.680%
32) Benzene-d6	8.276	84	633988	20.529	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.120%
36) 1,2-Dichloropropane-d6	9.270	67	195662	21.492	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.960%
41) Toluene-d8	10.319	98	569436	20.557	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.240%
43) trans-1,3-Dichloroprop...	10.575	79	81035	21.959	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.840%
47) 2-Hexanone-d5	10.922	63	69828	59.182	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	170221	26.837	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.360%
66) 1,2-Dichlorobenzene-d4	13.849	152	157805	22.318	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.280%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	8378	3.007	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
Data File : VW030946.D
Acq On : 06 Nov 2024 17:18
Operator : SY/MD
Sample : P4724-08
Misc : 5.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 07 03:59:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 07 03:58:00 2024
Response via : Initial Calibration

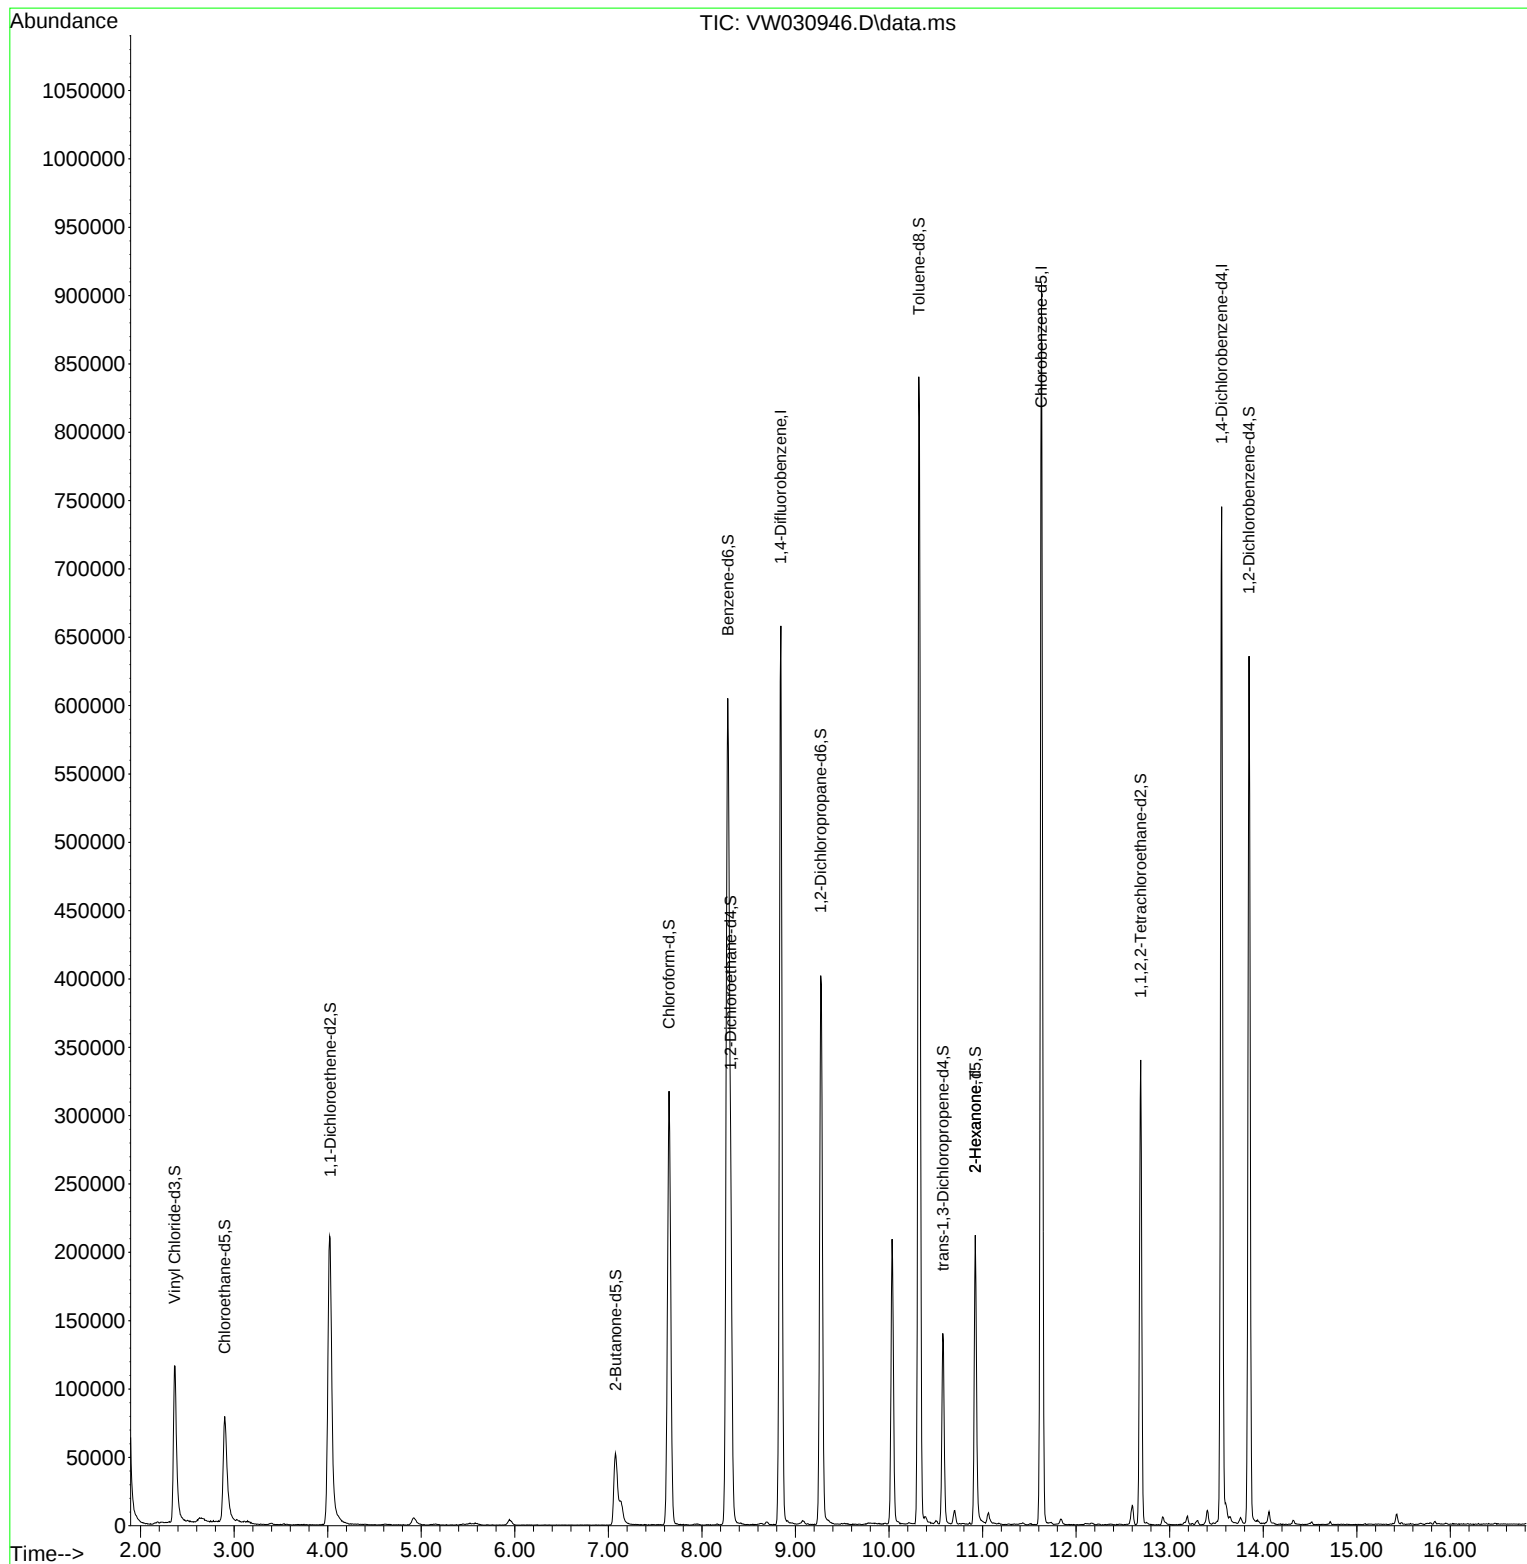

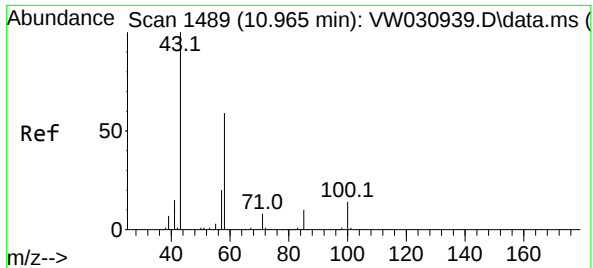

#48
 2-Hexanone
 Concen: 3.007 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW030946.D
 Acq: 06 Nov 2024 17:18

Instrument :
 MSVOA_W
 ClientSampleId :

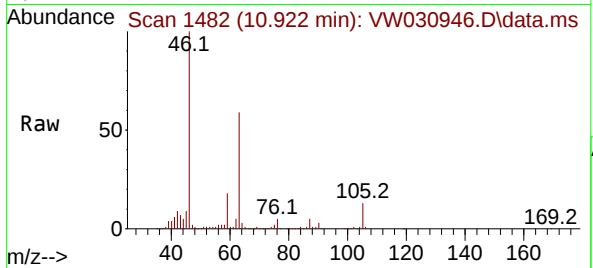

Tgt Ion: 43	Resp: 8378
Ion Ratio	Lower Upper
43	100
58	32.3 43.8 65.8#
57	36.2 15.4 23.2#
100	4.2 10.2 15.2#

