
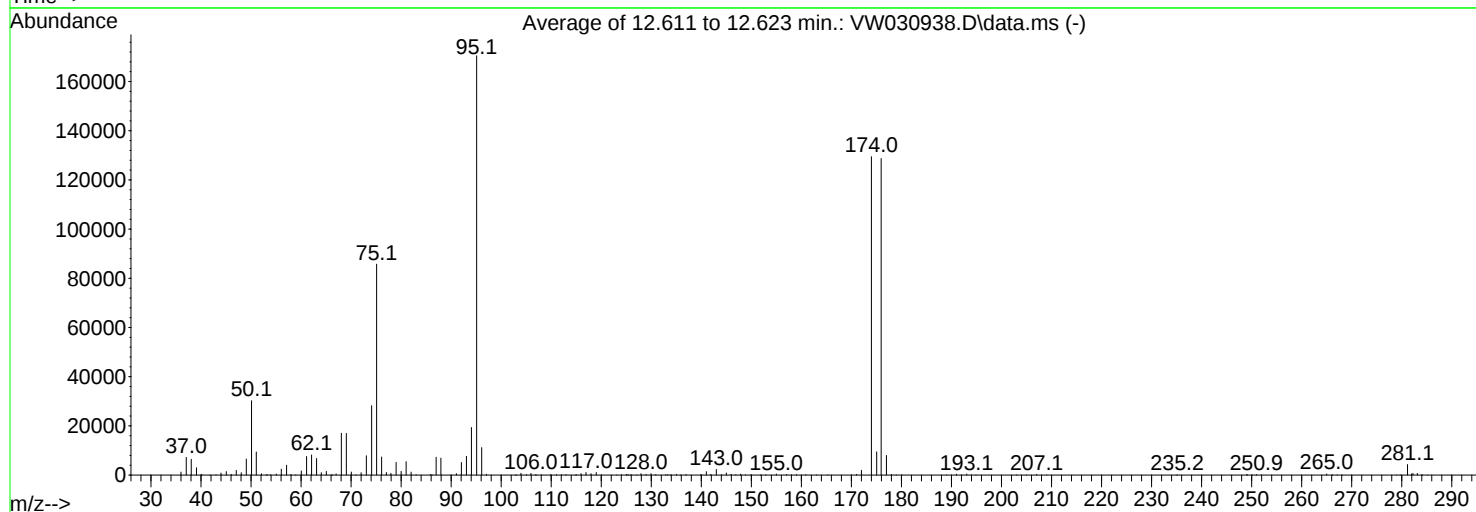


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110624\
Data File : VW030938.D
Acq On : 06 Nov 2024 08:46
Operator : SY/MD
Sample : BFB592
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB592

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Thu Nov 07 03:58:00 2024

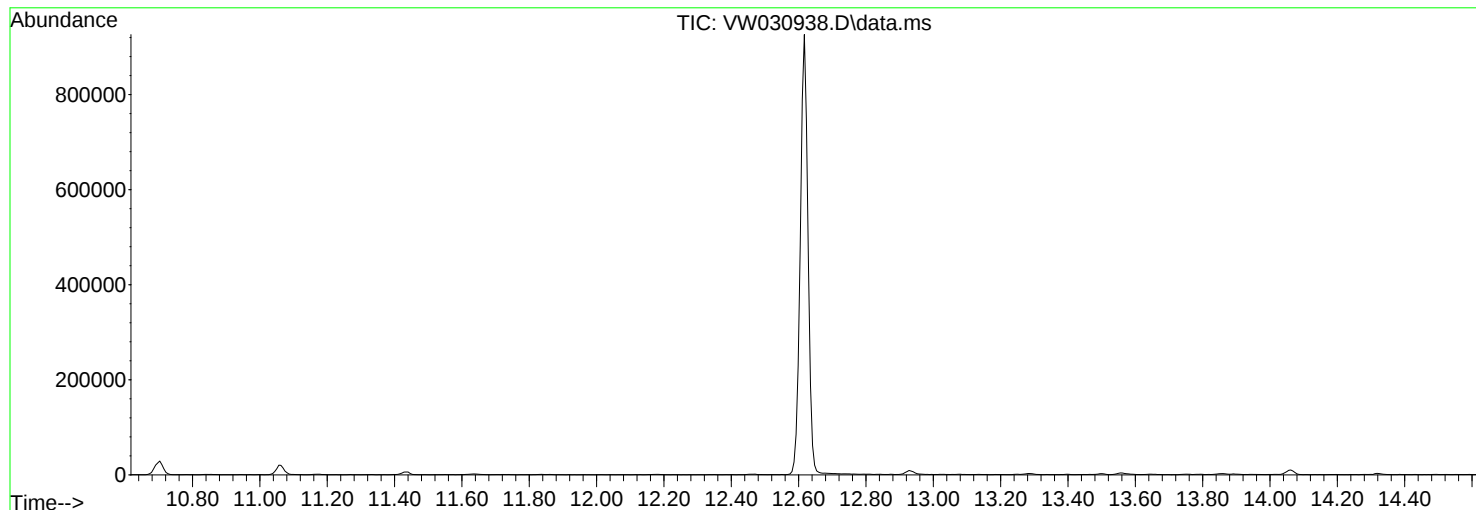

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	30253	PASS
75	95	30	80	50.3	85757	PASS
95	95	100	100	100.0	170496	PASS
96	95	5	9	6.6	11186	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.9	129443	PASS
175	174	5	9	7.3	9443	PASS
176	174	95	101	99.4	128717	PASS
177	176	5	9	6.2	7965	PASS

Scan 1751 (12.562 min): VW030938.D\data.ms
BFB592

m/z	Abundance
36.00	113.0
39.90	191.0
44.10	182.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

m/z	Abundance
36.10	1252.0
37.00	7792.0
38.00	6842.0
39.10	3057.0
40.20	360.0
43.10	141.0
44.00	945.0
45.10	1430.0
46.20	238.0
47.00	1942.0
48.00	952.0
49.10	6667.0
50.10	31232.0
51.00	9576.0
52.10	647.0
53.00	250.0
53.90	79.0
55.10	381.0
56.00	2750.0
57.10	4160.0
58.00	311.0
58.90	201.0
60.00	1646.0
61.10	7332.0
62.10	8218.0
63.10	7209.0
64.00	1140.0
65.00	1700.0
66.10	193.0
67.00	447.0
68.10	16856.0
69.10	17312.0
70.10	1368.0
71.00	84.0
72.00	1150.0
73.00	8144.0
74.10	27520.0
75.10	87048.0
76.10	7430.0
77.10	1183.0
77.90	639.0
79.00	5713.0
80.00	1608.0
81.00	5817.0
82.00	1278.0
83.00	120.0
86.00	254.0
87.00	7706.0
88.00	6910.0
91.00	544.0
92.10	4984.0
93.10	7537.0
94.10	19040.0
95.10	173120.0
96.10	11479.0
97.00	391.0
102.80	124.0
103.90	722.0
105.00	219.0
105.90	619.0
106.90	128.0
108.10	126.0
110.00	161.0
111.10	193.0
112.20	120.0
113.00	171.0
114.80	151.0
116.00	487.0
116.90	1088.0
118.00	595.0
119.00	1030.0
124.10	142.0
125.10	489.0
125.80	142.0
127.10	64.0
127.90	534.0
128.90	255.0
129.90	468.0
131.00	266.0
132.90	509.0
133.80	114.0
135.00	342.0
137.00	275.0
139.90	79.0
141.00	1206.0
141.90	180.0
143.00	2081.0
144.00	162.0
145.00	1086.0
145.90	291.0
147.00	240.0
148.00	311.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

149.00	124.0
149.90	219.0
151.70	59.0
153.00	57.0
155.10	407.0
157.00	337.0
159.10	185.0
161.00	171.0
163.00	95.0
165.30	62.0
170.00	82.0
171.00	354.0
172.00	2096.0
174.00	110072.0
175.00	8700.0
175.90	103520.0
177.00	7967.0
178.00	263.0
179.00	212.0
180.10	59.0
189.00	59.0
191.00	572.0
192.10	107.0
193.10	737.0
194.10	125.0
194.90	60.0
203.00	116.0
205.00	146.0
207.00	427.0
208.00	80.0
209.00	63.0
235.10	126.0
249.00	449.0
250.10	125.0
250.90	282.0
252.00	103.0
265.00	741.0
266.20	138.0
267.10	257.0
268.10	88.0
279.00	83.0
279.70	85.0
281.10	6819.0
282.20	1472.0
283.10	1313.0
284.00	269.0
285.20	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

m/z	Abundance
36.10	1632.0
37.10	7739.0
38.10	6995.0
39.10	3183.0
40.20	404.0
41.80	58.0
43.00	124.0
44.00	1198.0
45.10	1567.0
46.00	122.0
47.10	2120.0
48.10	1130.0
49.00	7146.0
50.10	33128.0
51.10	10562.0
52.10	549.0
53.10	278.0
53.90	71.0
55.10	481.0
56.10	2423.0
57.10	4401.0
58.00	192.0
59.00	102.0
60.00	1866.0
61.10	8788.0
62.10	9212.0
63.10	7293.0
64.10	1183.0
65.10	1658.0
66.30	115.0
67.00	518.0
68.10	19584.0
69.00	18112.0
70.00	1312.0
71.00	77.0
72.00	879.0
73.10	8605.0
74.10	32808.0
75.10	96288.0
76.10	8321.0
77.10	997.0
78.00	830.0
79.00	5368.0
80.00	1609.0
81.00	5625.0
82.00	1449.0
83.00	183.0
85.80	269.0
86.20	237.0
87.00	7461.0
88.00	7704.0
91.00	706.0
92.00	5473.0
93.10	8676.0
94.10	22272.0
95.10	184448.0
96.10	12304.0
97.10	309.0
103.10	193.0
104.00	893.0
105.10	244.0
106.00	769.0
106.70	158.0
107.10	185.0
108.10	118.0
109.80	175.0
111.00	231.0
112.00	166.0
112.90	177.0
115.00	178.0
116.00	807.0
117.00	1175.0
117.90	651.0
119.00	1237.0
120.10	82.0
123.10	61.0
124.00	99.0
124.90	264.0
125.40	126.0
126.20	108.0
128.00	676.0
129.00	395.0
130.00	618.0
130.80	186.0
133.30	379.0
135.10	290.0
136.90	243.0
139.80	132.0
141.00	1618.0
141.80	212.0
143.00	2766.0
145.00	978.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

145.90	309.0
146.90	130.0
147.80	365.0
148.80	114.0
150.00	192.0
151.80	77.0
152.90	118.0
154.90	401.0
157.00	259.0
158.00	90.0
159.10	207.0
160.90	263.0
163.10	96.0
165.30	66.0
171.10	323.0
172.00	2344.0
174.00	155328.0
175.10	10794.0
176.00	152064.0
177.00	8519.0
177.90	206.0
178.90	88.0
191.00	321.0
192.00	84.0
193.00	349.0
194.00	55.0
207.10	264.0
209.10	55.0
235.20	83.0
249.20	395.0
250.10	113.0
251.00	306.0
251.90	55.0
265.00	384.0
266.20	186.0
267.20	58.0
281.20	4081.0
281.90	886.0
282.30	732.0
283.10	538.0
284.20	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

m/z	Abundance
36.00	1135.0
37.10	6103.0
38.00	5450.0
39.10	2733.0
40.10	263.0
42.90	104.0
44.00	903.0
45.00	1284.0
46.00	228.0
47.00	1719.0
48.00	882.0
49.10	5831.0
50.10	26400.0
51.10	8053.0
52.10	404.0
52.90	91.0
53.30	100.0
53.90	54.0
54.90	439.0
56.10	2141.0
57.10	3462.0
58.10	141.0
60.10	1541.0
61.10	6567.0
62.10	7137.0
63.10	5706.0
64.00	652.0
65.10	1178.0
66.00	134.0
67.00	485.0
68.00	14609.0
69.00	15414.0
70.10	1106.0
70.90	92.0
72.00	890.0
73.00	6864.0
74.10	24304.0
75.10	73936.0
76.10	6334.0
77.00	1013.0
78.00	710.0
79.00	4406.0
80.00	1369.0
81.00	4979.0
82.00	959.0
82.90	101.0
85.90	161.0
87.00	6591.0
87.90	6029.0
91.10	519.0
92.10	4878.0
93.00	6707.0
94.00	16728.0
95.10	153920.0
96.10	9776.0
97.10	378.0
103.10	63.0
103.90	610.0
105.10	264.0
106.00	596.0
106.90	120.0
110.00	97.0
111.10	103.0
112.10	194.0
112.90	163.0
115.10	163.0
115.90	467.0
116.90	958.0
117.90	478.0
119.00	846.0
120.10	65.0
124.00	80.0
125.20	118.0
126.00	149.0
127.90	536.0
128.90	276.0
129.90	553.0
130.90	241.0
133.30	137.0
134.00	75.0
135.00	285.0
135.90	70.0
137.00	238.0
140.10	160.0
141.00	1384.0
142.00	195.0
143.00	2005.0
144.10	102.0
145.00	542.0
146.00	319.0
146.80	102.0
147.80	321.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592

148.80	138.0
150.00	85.0
151.90	120.0
152.90	190.0
155.00	483.0
157.10	244.0
158.00	80.0
159.00	196.0
160.80	115.0
171.00	246.0
172.00	1507.0
174.00	122928.0
175.10	8835.0
176.00	130568.0
177.00	7409.0
178.10	276.0
191.00	169.0
193.00	195.0
193.90	74.0
207.00	141.0
234.90	67.0
249.10	171.0
250.90	91.0
265.00	223.0
266.00	53.0
281.10	1928.0
282.00	511.0
283.10	268.0

Instrument :
MSVOA_W
ClientSampleId :
BFB592