

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110724\
 Data File : VW030951.D
 Acq On : 07 Nov 2024 10:39
 Operator : SY/MD
 Sample : VW1107SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 04:05:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 04:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	462808	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	437116	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	186478	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	142998	18.839	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.360%
7) Chloroethane-d5	2.905	69	115610	19.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.440%
11) 1,1-Dichloroethene-d2	4.021	65	63900	20.402	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.600%
21) 2-Butanone-d5	7.081	46	58679	46.976	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.960%
24) Chloroform-d	7.648	84	309967	22.719	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.880%
26) 1,2-Dichloroethane-d4	8.307	65	158565	23.375	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.480%
32) Benzene-d6	8.276	84	599832	22.089	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.360%
36) 1,2-Dichloropropane-d6	9.276	67	184232	23.014	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.040%
41) Toluene-d8	10.325	98	546399	22.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.720%
43) trans-1,3-Dichloroprop...	10.575	79	68773	21.194	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.760%
47) 2-Hexanone-d5	10.922	63	48235	46.492	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	131703	23.614	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.440%
66) 1,2-Dichlorobenzene-d4	13.855	152	174431	25.679	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4732	0.449	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110724\
Data File : VW030951.D
Acq On : 07 Nov 2024 10:39
Operator : SY/MD
Sample : VW1107SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 08 04:05:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 04:04:29 2024
Response via : Initial Calibration

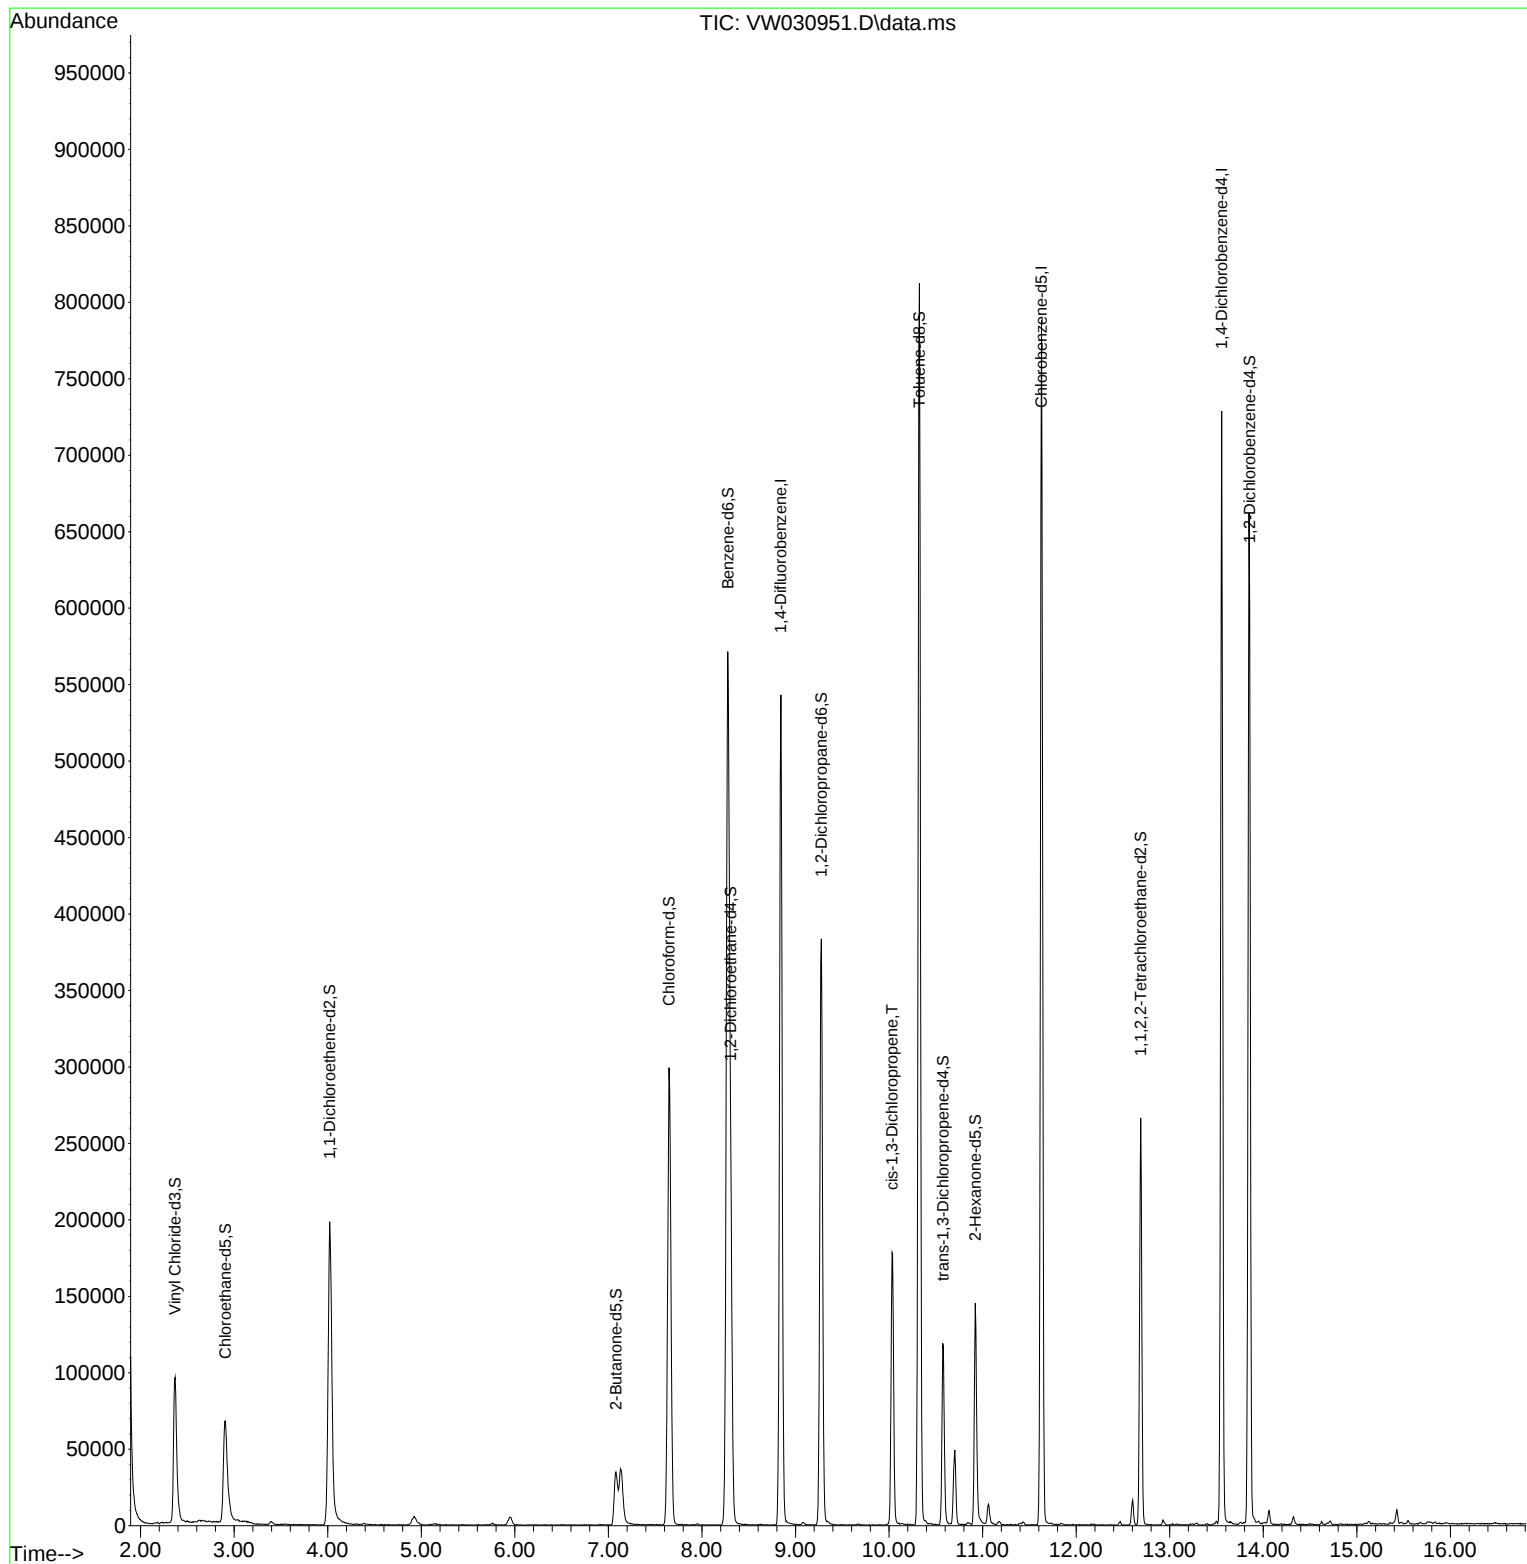

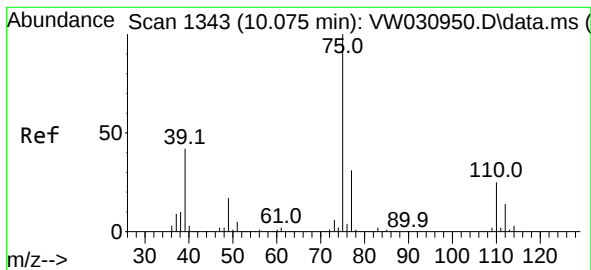

#39
 cis-1,3-Dichloropropene
 Concen: 0.449 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW030951.D
 Acq: 07 Nov 2024 10:39

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4732
 Ion Ratio Lower Upper
 75 100
 77 48.1 21.3 39.6#

