
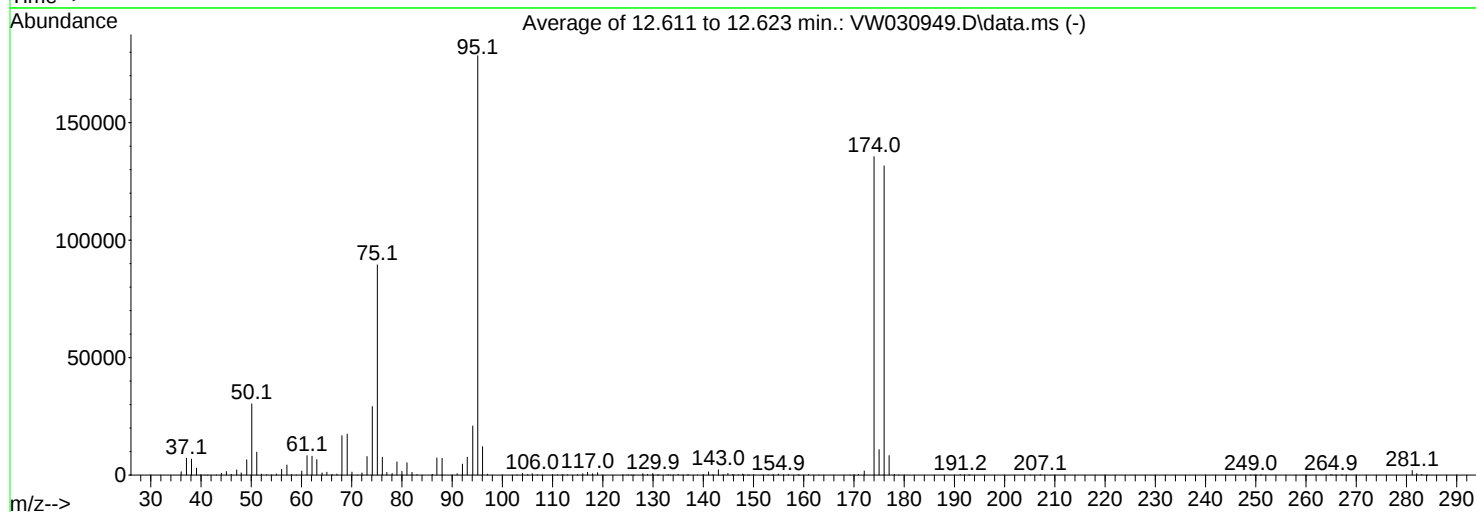


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110724\
Data File : VW030949.D
Acq On : 07 Nov 2024 08:55
Operator : SY/MD
Sample : BFB593
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB593

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Fri Nov 08 04:04:29 2024

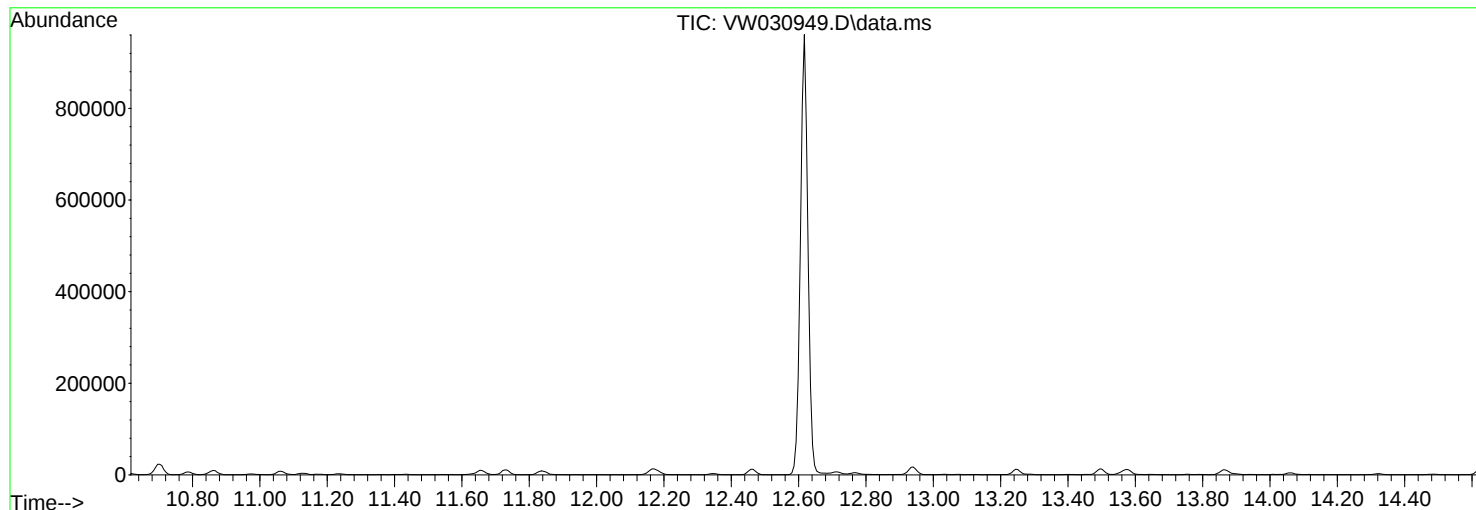

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	30333	PASS
75	95	30	80	50.1	89501	PASS
95	95	100	100	100.0	178496	PASS
96	95	5	9	6.8	12104	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.9	135512	PASS
175	174	5	9	8.0	10831	PASS
176	174	95	101	97.1	131627	PASS
177	176	5	9	6.3	8302	PASS

m/z	Abundance
40.00	243.0
44.10	269.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

m/z	Abundance
36.00	1413.0
37.10	7838.0
38.10	7175.0
39.10	3193.0
40.20	360.0
41.30	52.0
43.10	90.0
44.00	972.0
45.10	1617.0
46.10	218.0
47.10	2251.0
48.00	942.0
49.10	6474.0
50.10	31152.0
51.10	9822.0
52.10	462.0
53.00	229.0
54.20	121.0
55.00	444.0
56.10	2191.0
57.10	4407.0
58.10	151.0
59.00	96.0
60.10	1610.0
61.10	8259.0
62.10	8350.0
63.10	7053.0
64.10	1276.0
65.00	1509.0
66.10	225.0
67.00	415.0
68.00	17064.0
69.10	17664.0
70.10	1187.0
71.20	68.0
72.10	994.0
73.10	7935.0
74.10	29040.0
75.10	88528.0
76.10	7965.0
76.90	1227.0
78.20	702.0
79.00	5775.0
80.00	1544.0
81.00	5495.0
81.90	1149.0
83.00	176.0
86.00	312.0
87.00	7647.0
88.00	7198.0
91.00	557.0
92.10	4537.0
93.00	7702.0
94.10	21024.0
95.10	169856.0
96.10	12103.0
97.00	435.0
102.90	165.0
103.90	811.0
105.00	304.0
106.00	555.0
106.90	134.0
107.90	66.0
110.10	152.0
111.00	184.0
111.90	126.0
113.10	137.0
114.90	203.0
116.00	625.0
117.00	1275.0
117.90	546.0
119.00	963.0
124.00	130.0
124.80	175.0
125.20	172.0
126.20	81.0
127.90	516.0
129.00	227.0
130.00	652.0
131.20	171.0
133.10	227.0
135.00	256.0
135.80	89.0
136.80	263.0
138.90	94.0
141.00	1204.0
142.00	205.0
143.00	2423.0
143.90	285.0
144.90	679.0
145.90	188.0
147.10	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

147.80	310.0
148.10	301.0
148.90	126.0
150.10	76.0
151.90	127.0
152.90	193.0
153.70	51.0
155.00	345.0
156.00	61.0
156.90	258.0
158.90	289.0
160.90	220.0
163.00	114.0
169.20	57.0
170.90	471.0
172.00	1790.0
174.00	120728.0
175.00	9111.0
176.00	117376.0
177.00	7292.0
178.10	298.0
178.90	92.0
191.20	313.0
191.90	66.0
192.90	317.0
205.10	70.0
207.20	229.0
249.00	133.0
250.10	66.0
251.00	74.0
251.20	74.0
264.90	452.0
266.00	129.0
267.10	116.0
268.10	60.0
281.20	2782.0
282.00	872.0
283.00	575.0
284.20	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

m/z	Abundance
36.10	1538.0
37.10	8313.0
38.10	8068.0
39.10	3139.0
40.00	289.0
43.00	134.0
44.00	1233.0
45.10	1793.0
46.00	300.0
47.10	2237.0
48.10	1171.0
49.10	7469.0
50.10	33520.0
51.10	10983.0
52.00	452.0
53.10	135.0
54.00	110.0
55.00	473.0
56.10	2958.0
57.10	4847.0
58.00	220.0
59.00	82.0
60.10	2192.0
61.10	9439.0
62.10	9260.0
63.00	6976.0
64.10	846.0
65.00	1249.0
66.10	205.0
67.10	462.0
68.10	19144.0
69.10	19960.0
70.10	1705.0
71.10	86.0
72.00	886.0
73.00	8706.0
74.10	32648.0
75.10	102208.0
76.10	8169.0
77.00	1262.0
78.00	734.0
79.00	6226.0
80.00	1898.0
81.00	5973.0
82.00	1395.0
83.00	249.0
86.10	265.0
87.00	8403.0
88.00	7878.0
91.00	724.0
92.00	5526.0
93.00	8474.0
94.10	23224.0
95.10	208512.0
96.10	13900.0
97.10	361.0
102.90	137.0
104.00	752.0
105.00	329.0
105.90	738.0
106.90	186.0
110.00	165.0
110.80	100.0
111.10	85.0
112.10	147.0
112.90	162.0
114.90	234.0
116.00	618.0
117.00	1323.0
118.00	686.0
118.90	1297.0
124.10	114.0
125.10	92.0
125.80	125.0
127.90	647.0
128.90	420.0
129.90	611.0
130.90	320.0
132.80	190.0
133.50	103.0
134.10	67.0
135.00	338.0
137.00	322.0
138.80	82.0
140.00	187.0
141.10	1630.0
141.90	238.0
143.00	2498.0
144.00	146.0
145.00	810.0
145.80	345.0
146.90	232.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

147.90	627.0
148.90	173.0
150.00	146.0
151.80	72.0
152.90	89.0
153.90	153.0
154.90	565.0
156.00	81.0
157.00	312.0
158.90	312.0
161.00	207.0
170.10	65.0
171.00	307.0
172.00	1776.0
174.00	157568.0
175.00	12575.0
176.00	145728.0
177.00	10196.0
178.00	326.0
178.90	95.0
191.10	261.0
192.00	99.0
193.10	162.0
205.20	53.0
207.00	158.0
249.00	149.0
265.20	245.0
265.90	59.0
267.30	78.0
281.10	2214.0
282.10	757.0
283.10	267.0
284.20	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

m/z	Abundance
36.10	1318.0
37.10	5480.0
38.10	5239.0
39.10	2656.0
40.00	286.0
40.80	58.0
43.10	100.0
44.10	749.0
45.00	1171.0
46.00	152.0
47.10	2109.0
47.90	735.0
49.10	5570.0
50.10	26328.0
51.10	8559.0
52.00	292.0
53.00	155.0
55.00	420.0
56.00	2088.0
57.10	3650.0
58.00	184.0
58.80	90.0
60.00	1356.0
61.10	7074.0
62.10	6467.0
63.10	5788.0
64.00	675.0
65.10	990.0
66.10	226.0
67.10	448.0
68.10	14142.0
69.10	14760.0
70.00	1018.0
71.00	125.0
72.10	830.0
73.00	7031.0
74.10	25832.0
75.10	77768.0
76.10	6694.0
77.10	917.0
78.00	574.0
79.00	4825.0
80.00	1388.0
81.00	4302.0
82.10	943.0
82.90	131.0
86.10	291.0
86.90	5782.0
88.00	6406.0
91.00	501.0
92.00	3960.0
93.00	6692.0
94.10	18464.0
95.10	157120.0
96.00	10310.0
97.10	344.0
103.00	100.0
104.10	595.0
105.10	235.0
105.90	510.0
107.00	179.0
109.90	112.0
111.10	93.0
111.90	131.0
112.90	157.0
115.00	224.0
116.00	528.0
116.80	897.0
117.90	495.0
119.00	850.0
123.90	96.0
125.70	105.0
128.00	583.0
128.80	272.0
130.00	685.0
131.10	211.0
133.10	80.0
135.00	319.0
137.00	256.0
140.00	185.0
141.10	1290.0
141.90	160.0
143.00	1826.0
143.90	87.0
144.80	502.0
146.10	232.0
147.10	121.0
147.90	373.0
148.90	89.0
149.20	93.0
150.00	114.0
152.00	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593

152.90	128.0
154.00	125.0
154.90	370.0
156.00	88.0
157.00	228.0
159.10	140.0
160.90	271.0
170.10	56.0
170.80	179.0
172.10	1657.0
174.00	128240.0
175.00	10808.0
176.00	131776.0
177.00	7417.0
178.00	192.0
191.00	85.0
193.00	90.0
207.00	97.0
249.70	54.0
250.90	73.0
265.00	153.0
281.00	924.0
282.10	244.0

Instrument :
MSVOA_W
ClientSampleId :
BFB593