

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110821\
 Data File : VW020801.D
 Acq On : 08 Nov 2021 10:55
 Operator : SY/VA
 Sample : M4511-06RE
 Misc : 6.47g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 09 07:10:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:39:29 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	197461	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	171508	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	91166	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	52859	28.471	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	113.880%
7) Chloroethane-d5	2.885	69	29557	27.959	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.840%
11) 1,1-Dichloroethene-d2	4.013	63	68110	17.478	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.920%
21) 2-Butanone-d5	7.080	46	20979	34.025	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.060%
24) Chloroform-d	7.647	84	98931	22.548	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	8.305	65	50130	21.463	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.840%
32) Benzene-d6	8.275	84	200394	25.861	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.440%
36) 1,2-Dichloropropane-d6	9.274	67	58196	24.257	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.040%
41) Toluene-d8	10.323	98	196676	26.089	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.360%
43) trans-1,3-Dichloroprop...	10.579	79	26011	21.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.440%
47) 2-Hexanone-d5	10.920	63	17204	35.441	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	141.760%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	37992	19.108	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	67183	23.449	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.800%
Target Compounds						
13) Acetone	4.123	43	3434	5.985	ug/L	98
34) Trichloroethene	8.842	95	6035	2.207	ug/L #	5
35) Methylcyclohexane	9.274	83	14466	3.032	ug/L #	15
37) 1,2-Dichloropropane	9.274	63	6866	2.823	ug/L #	88
39) cis-1,3-Dichloropropene	10.030	75	2381	0.602	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110821\
Data File : VW020801.D
Acq On : 08 Nov 2021 10:55
Operator : SY/VA
Sample : M4511-06RE
Misc : 6.47g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 09 07:10:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Nov 08 04:39:29 2021
Response via : Initial Calibration




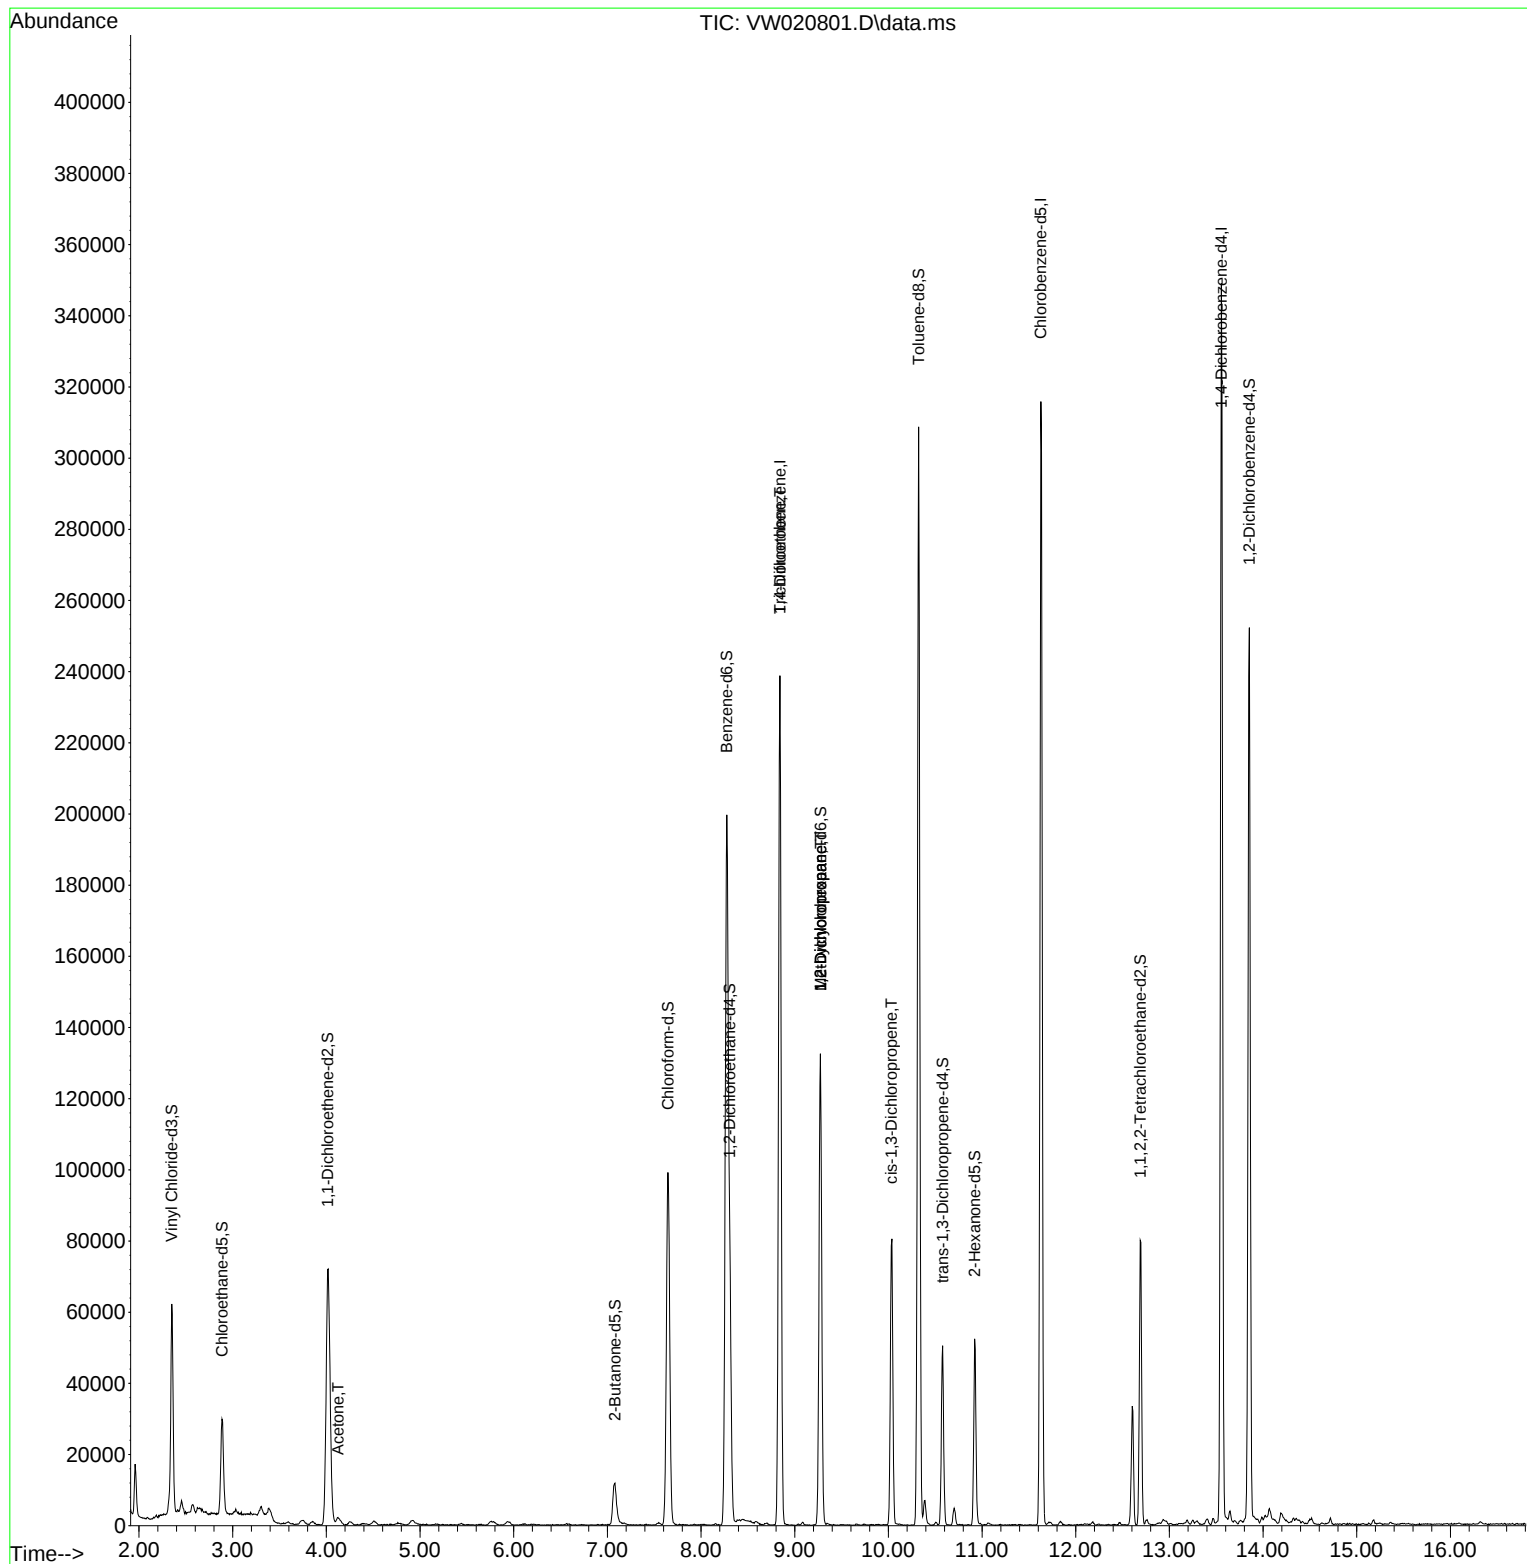


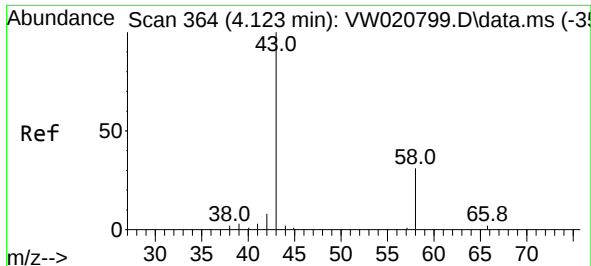

#13
Acetone
Concen: 5.985 ug/L
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW020801.D
Acq: 08 Nov 2021 10:55




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 3434
Ion Ratio Lower Upper
43 100
58 27.6 0.0 52.8

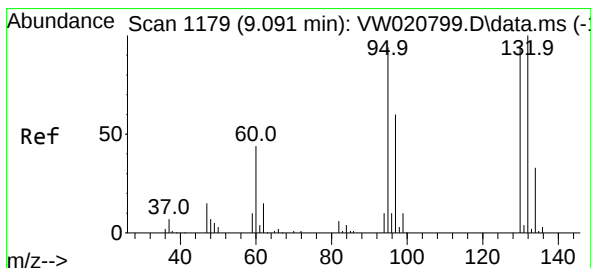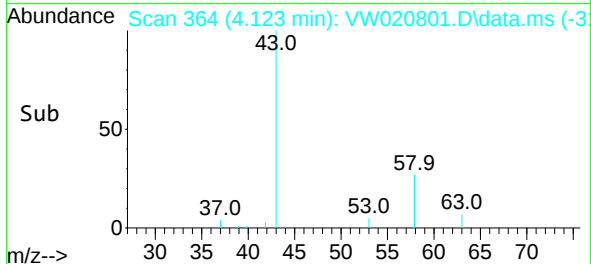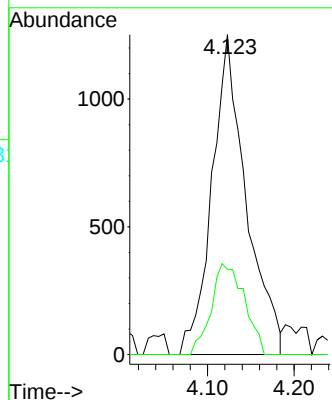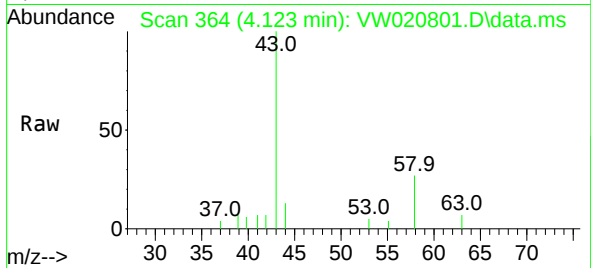

#34
Trichloroethene
Concen: 2.207 ug/L
RT: 8.842 min Scan# 1138
Delta R.T. -0.250 min
Lab File: VW020801.D
Acq: 08 Nov 2021 10:55

Tgt Ion: 95 Resp: 6035
Ion Ratio Lower Upper
95 100
97 0.0 47.0 87.2#
132 0.0 65.5 121.6#
130 0.0 69.4 128.8#


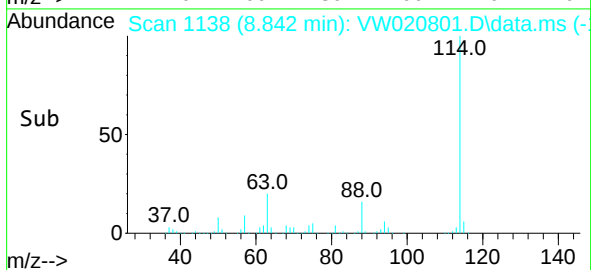
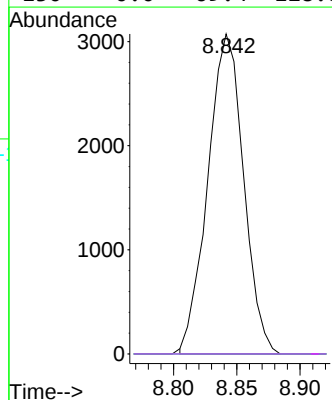
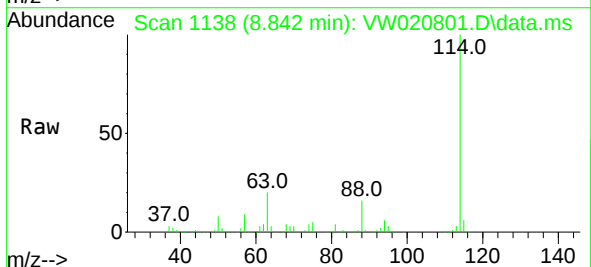


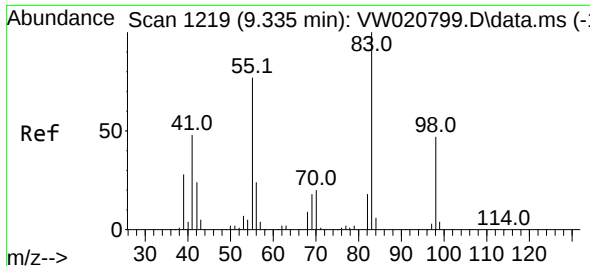

#35
Methylcyclohexane
Concen: 3.032 ug/L
RT: 9.274 min Scan# 11
Delta R.T. -0.061 min
Lab File: VW020801.D
Acq: 08 Nov 2021 10:55




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 14466
Ion Ratio Lower Upper
83 100
55 0.9 70.8 106.2#
98 1.8 37.7 56.5#

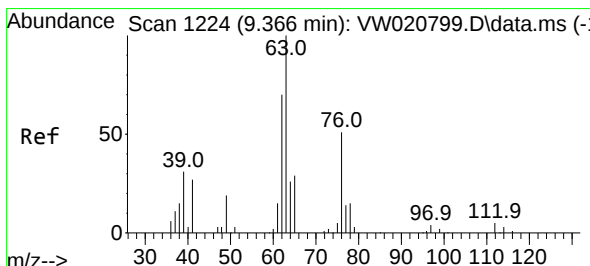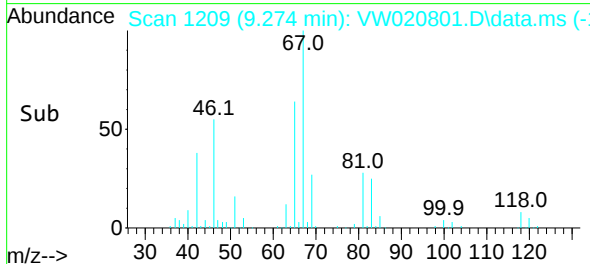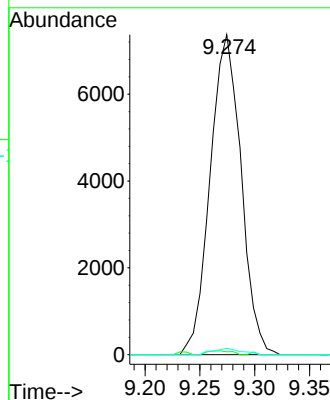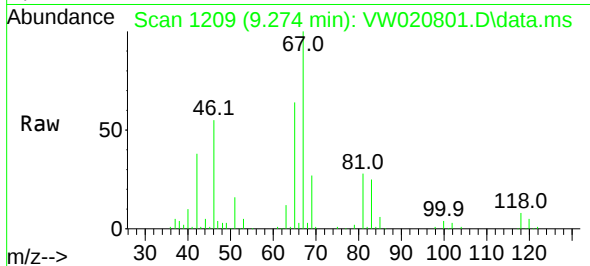

#37
1,2-Dichloropropane
Concen: 2.823 ug/L
RT: 9.274 min Scan# 1209
Delta R.T. -0.098 min
Lab File: VW020801.D
Acq: 08 Nov 2021 10:55


Tgt Ion: 63 Resp: 6866
Ion Ratio Lower Upper
63 100
112 0.0 3.2 4.8#

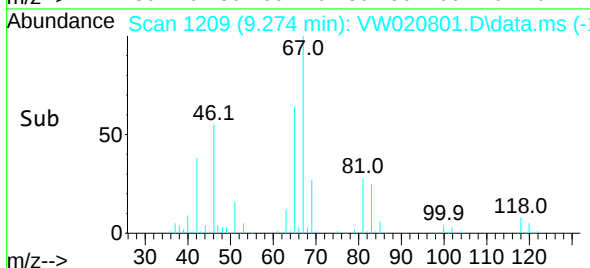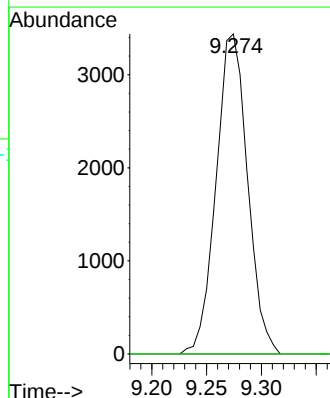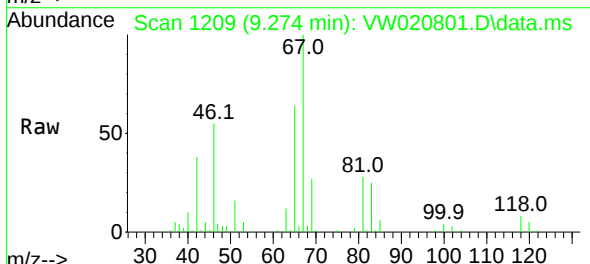

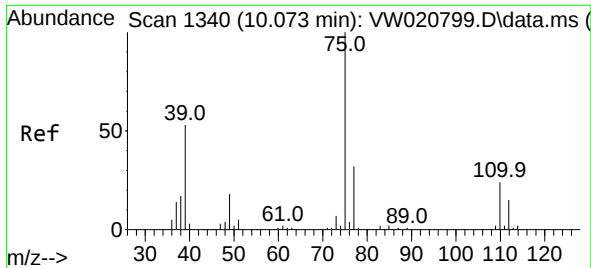

#39
 cis-1,3-Dichloropropene
 Concen: 0.602 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW020801.D
 Acq: 08 Nov 2021 10:55

Instrument :
 MSVOA_W
 ClientSampleId :

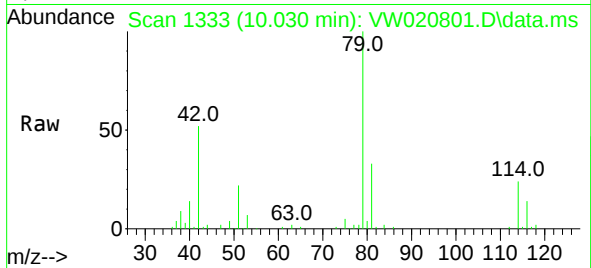

Tgt Ion: 75 Resp: 2381
 Ion Ratio Lower Upper
 75 100
 77 47.8 21.8 40.6#

