


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110821\
 Data File : VW020798.D
 Acq On : 08 Nov 2021 08:09
 Operator : SY/VA
 Sample : BFB460
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB460

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Title : SFAM01.0
 Last Update : Mon Nov 15 03:01:39 2021

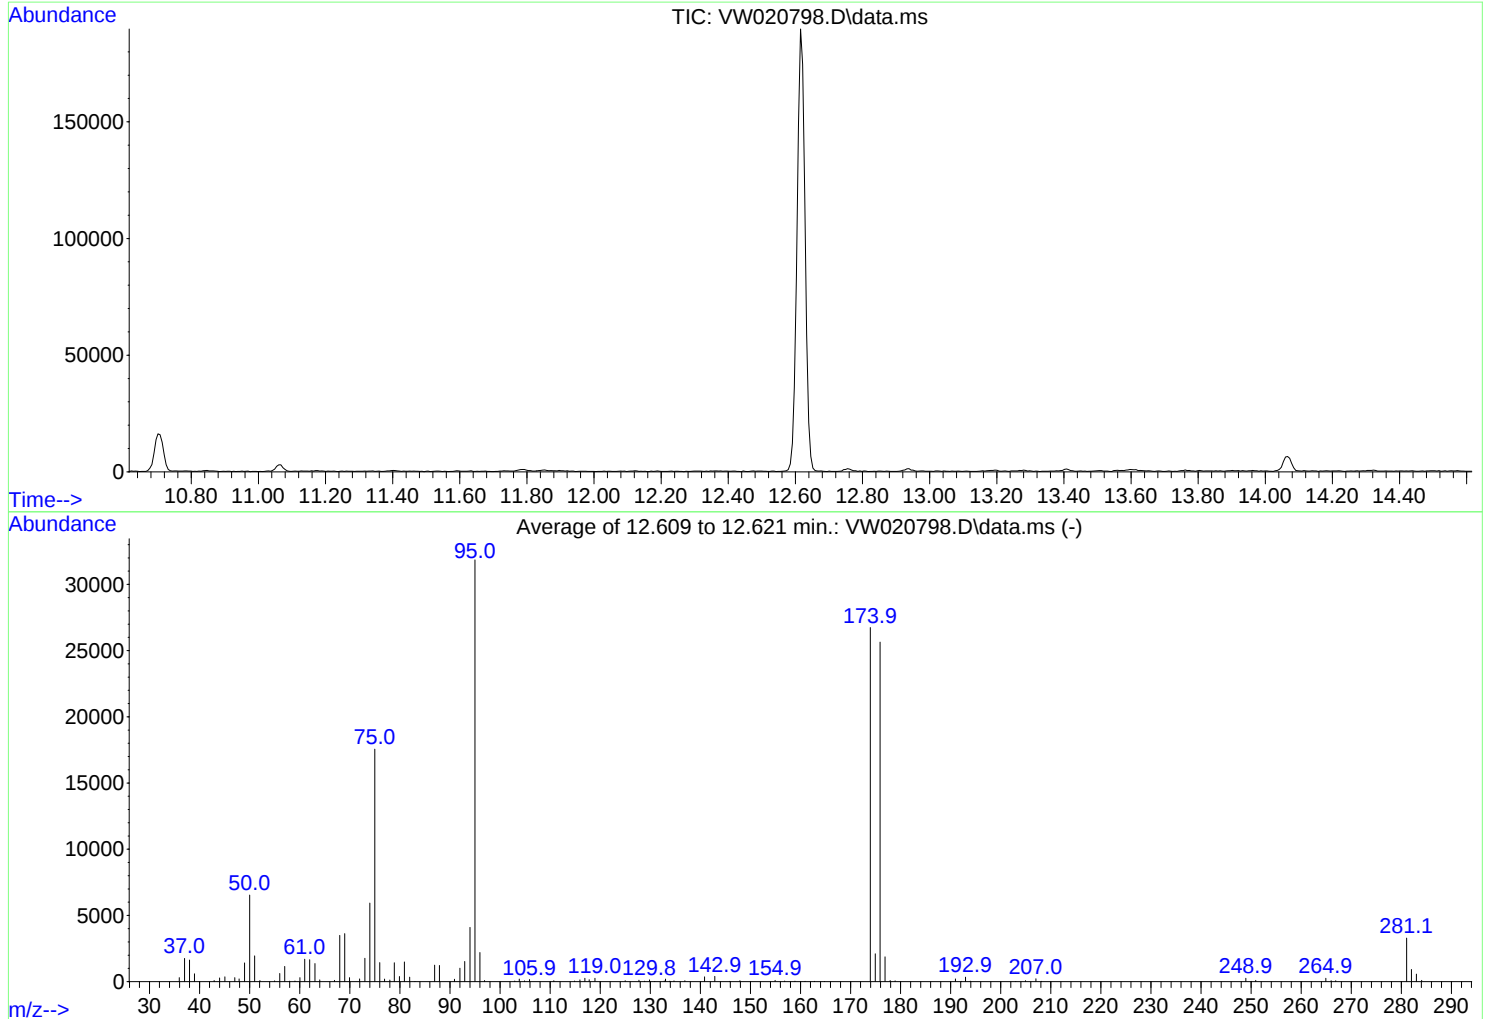

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	6543	PASS
75	95	30	80	55.1	17553	PASS
95	95	100	100	100.0	31853	PASS
96	95	5	9	6.9	2203	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	26747	PASS
175	174	5	9	7.9	2102	PASS
176	174	95	105	95.9	25645	PASS
177	176	5	10	7.3	1874	PASS

m/z	Abundance
40.00	80.0
40.90	97.0
44.00	89.0
55.10	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.00	302.0
37.00	1655.0
38.00	1437.0
39.00	584.0
40.00	85.0
41.00	59.0
42.90	94.0
44.00	344.0
45.00	372.0
47.10	253.0
47.90	157.0
49.00	1275.0
50.00	5934.0
51.00	1665.0
52.10	103.0
55.00	123.0
56.00	491.0
57.00	1034.0
58.00	59.0
59.00	88.0
60.00	239.0
61.00	1408.0
62.00	1460.0
63.10	1275.0
64.00	143.0
66.90	78.0
68.00	3024.0
69.00	3251.0
69.90	272.0
71.90	181.0
73.00	1705.0
74.00	5118.0
75.00	14907.0
76.00	1232.0
76.90	144.0
78.10	104.0
78.90	1218.0
79.90	316.0
80.90	1301.0
81.90	335.0
87.00	1226.0
87.90	1029.0
90.90	169.0
92.00	809.0
92.90	1306.0
94.00	3403.0
95.00	27816.0
96.00	1829.0
96.90	87.0
103.00	82.0
103.90	177.0
105.80	120.0
110.70	82.0
114.90	73.0
116.00	112.0
116.90	205.0
117.80	188.0
118.90	217.0
125.00	169.0
127.70	90.0
128.90	54.0
129.90	113.0
133.10	364.0
133.90	110.0
134.70	56.0
136.90	53.0
140.80	358.0
142.90	318.0
145.90	68.0
147.90	66.0
155.10	90.0
160.90	64.0
162.80	64.0
164.80	52.0
173.90	20176.0
174.90	1772.0
175.90	20312.0
176.90	1564.0
178.00	97.0
179.00	115.0
191.00	311.0
192.10	80.0
193.00	487.0
193.90	122.0
203.00	53.0
204.90	110.0
207.00	375.0
208.10	81.0
249.00	347.0
250.00	81.0
250.90	169.0
264.90	415.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

265.90	128.0
266.90	113.0
281.00	4876.0
282.00	1247.0
283.00	745.0
284.00	167.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.00	314.0
37.00	1837.0
38.00	1791.0
39.00	654.0
40.00	73.0
41.00	90.0
42.90	87.0
44.00	415.0
45.10	349.0
47.00	364.0
47.90	241.0
49.00	1639.0
50.00	7401.0
51.00	2342.0
52.10	68.0
55.00	89.0
56.00	738.0
57.00	1268.0
58.00	64.0
59.10	56.0
60.00	346.0
61.00	1892.0
62.00	1794.0
63.00	1513.0
64.00	201.0
67.00	101.0
68.00	3956.0
69.00	4078.0
70.00	330.0
72.00	186.0
73.00	2053.0
74.00	6830.0
75.00	19832.0
76.00	1616.0
77.00	245.0
78.00	149.0
78.90	1578.0
79.90	413.0
80.90	1709.0
81.90	354.0
87.00	1253.0
87.90	1357.0
90.80	171.0
92.00	1106.0
93.00	1587.0
94.00	4687.0
95.00	34864.0
96.00	2441.0
96.90	68.0
102.90	61.0
103.90	232.0
104.90	95.0
105.90	189.0
110.80	79.0
114.90	73.0
115.90	166.0
116.90	262.0
117.80	150.0
118.90	323.0
125.00	68.0
127.80	112.0
129.80	145.0
132.90	207.0
134.10	54.0
134.80	58.0
136.90	75.0
140.90	359.0
142.90	478.0
147.90	71.0
154.90	115.0
156.90	77.0
158.90	53.0
173.90	30320.0
174.90	2179.0
175.90	28544.0
176.90	1940.0
177.90	83.0
178.80	72.0
190.90	200.0
192.90	358.0
205.00	94.0
207.00	162.0
248.90	286.0
250.90	75.0
264.90	249.0
266.00	52.0
266.90	63.0
281.10	3268.0
282.00	958.0
283.10	667.0
284.10	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
35.90	278.0
37.00	1769.0
38.00	1661.0
39.00	549.0
40.00	71.0
40.90	86.0
42.90	61.0
44.00	346.0
45.00	355.0
47.00	293.0
47.90	221.0
49.00	1332.0
50.00	6293.0
51.00	1828.0
51.90	80.0
55.00	119.0
56.00	615.0
57.00	1140.0
60.10	319.0
61.00	1757.0
62.00	1709.0
63.00	1314.0
64.10	74.0
67.00	117.0
68.00	3513.0
69.00	3532.0
70.00	323.0
71.90	244.0
73.00	1548.0
74.00	5870.0
75.00	17920.0
76.00	1464.0
77.00	206.0
77.90	118.0
78.90	1502.0
79.90	436.0
80.90	1443.0
82.00	333.0
83.00	53.0
86.90	1264.0
87.90	1263.0
91.00	188.0
92.00	1118.0
93.00	1672.0
94.00	4217.0
95.00	32880.0
96.00	2338.0
96.90	88.0
103.80	176.0
104.90	83.0
106.00	176.0
110.70	56.0
115.90	107.0
117.00	282.0
117.90	110.0
119.00	220.0
127.80	130.0
128.90	50.0
129.90	130.0
130.90	55.0
132.80	132.0
134.80	72.0
136.90	90.0
140.90	388.0
142.90	393.0
147.90	68.0
154.90	96.0
156.80	82.0
158.90	53.0
174.00	29744.0
175.00	2355.0
175.90	28080.0
176.90	2119.0
177.80	65.0
191.00	112.0
192.90	159.0
206.90	129.0
248.90	122.0
250.90	50.0
265.00	115.0
266.00	56.0
267.00	51.0
281.00	1721.0
282.00	547.0
282.90	312.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460