



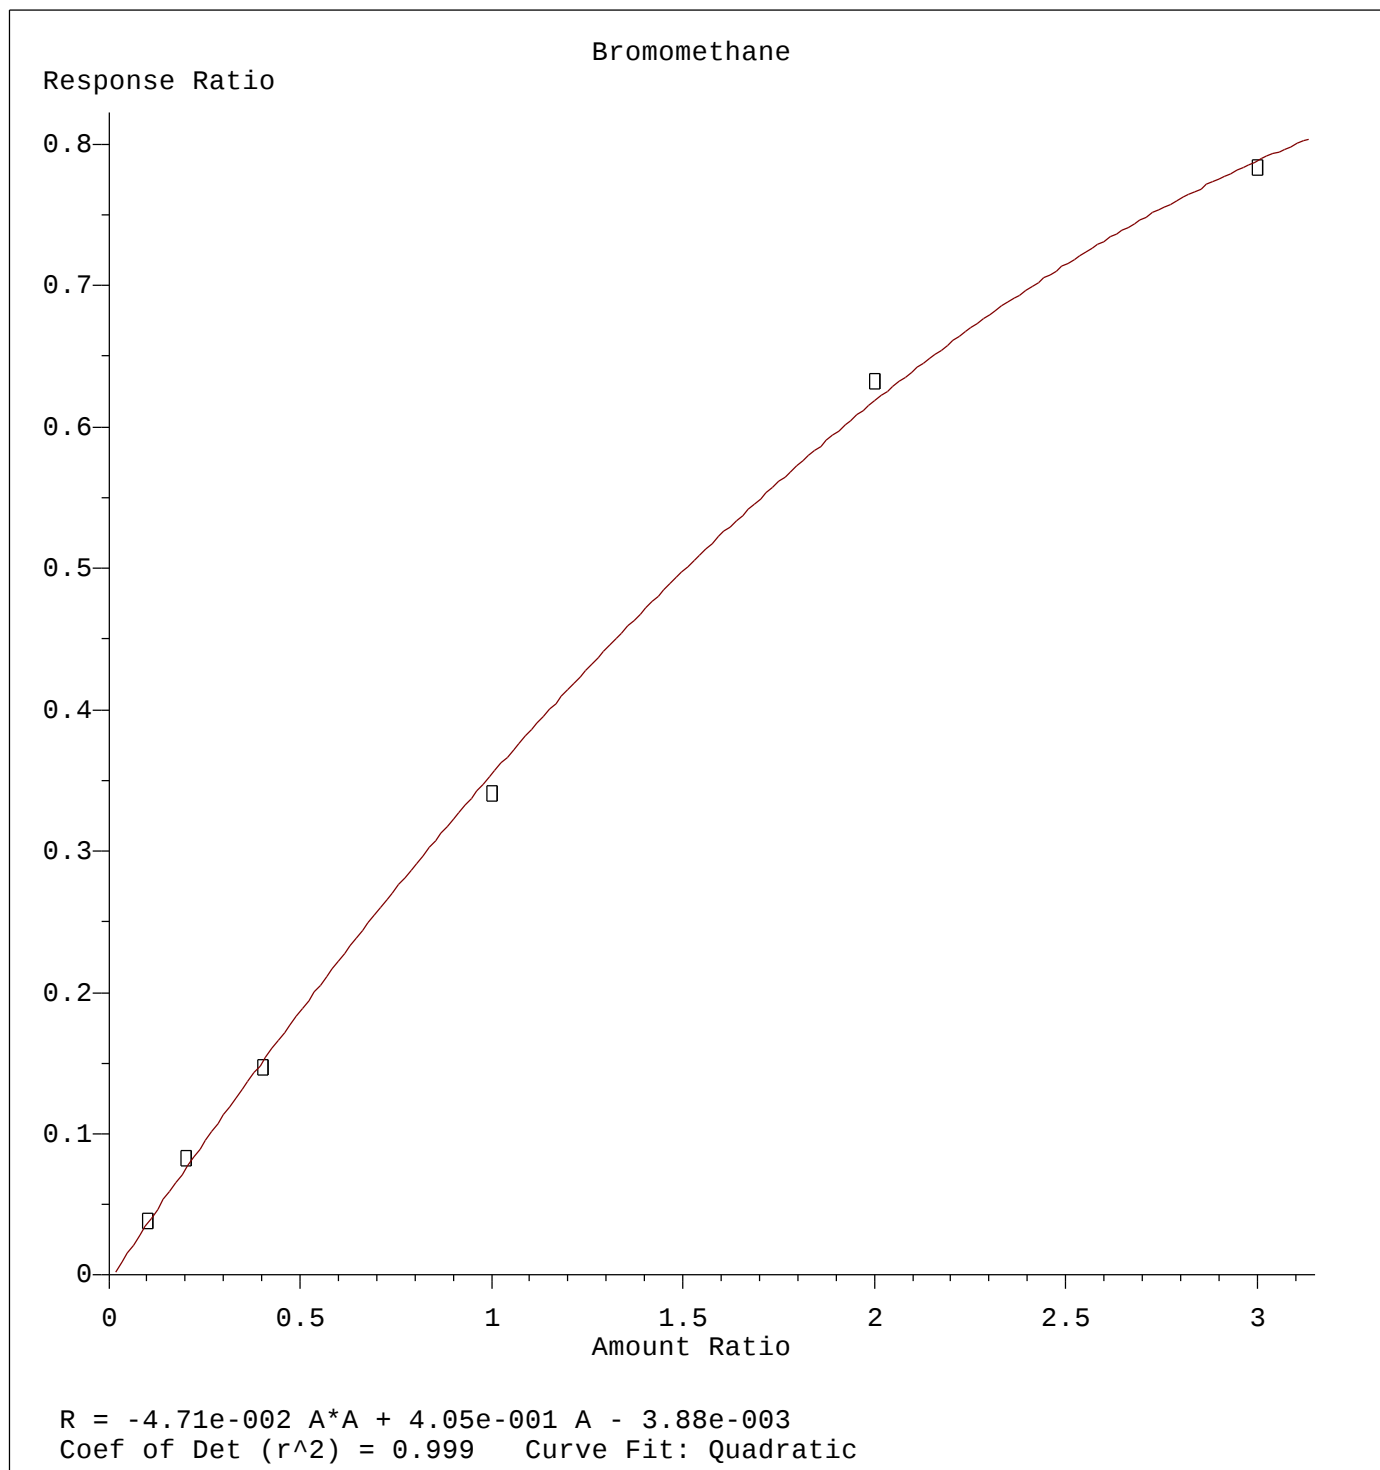

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W110918S.M  
Calibration Table Last Updated: Mon Nov 12 17:15:47 2018

# Methylene Chloride

Response Ratio

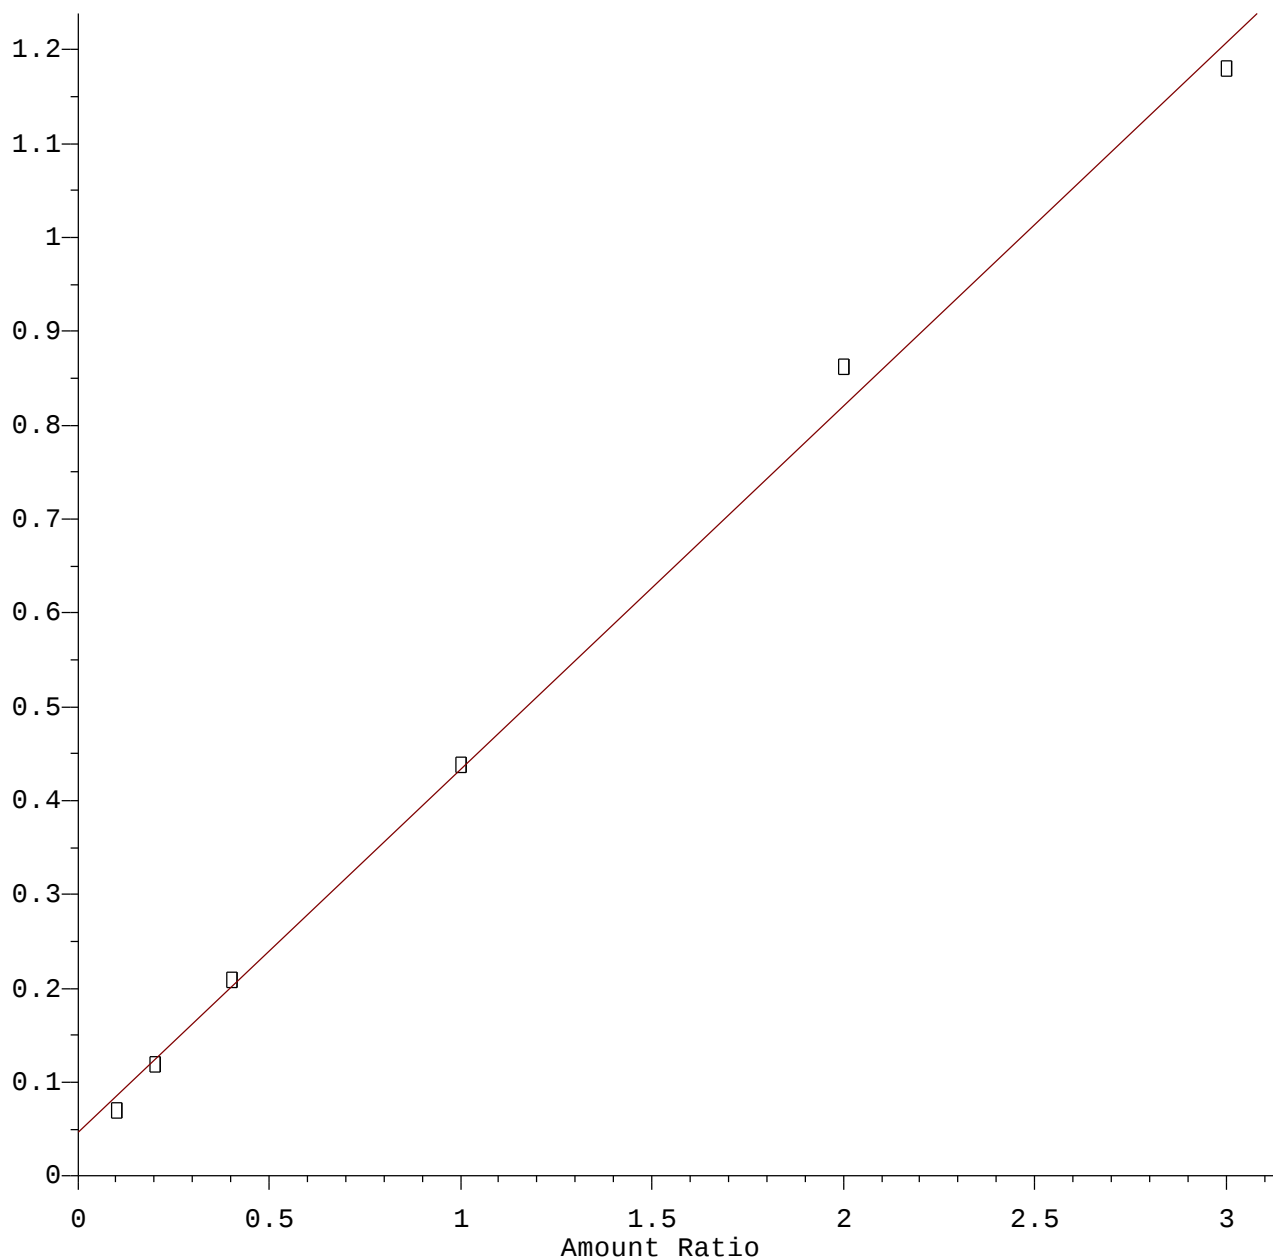

Resp Ratio =  $3.87 \times 10^{-1} \times \text{Amt} + 4.75 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W110918S.M  
Calibration Table Last Updated: Mon Nov 12 17:15:47 2018