


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110918\
Data File : VW006781.D
Acq On : 09 Nov 2018 11:12
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110918S.M
Title : SW846 8260
Last Update : Mon Nov 12 00:52:45 2018

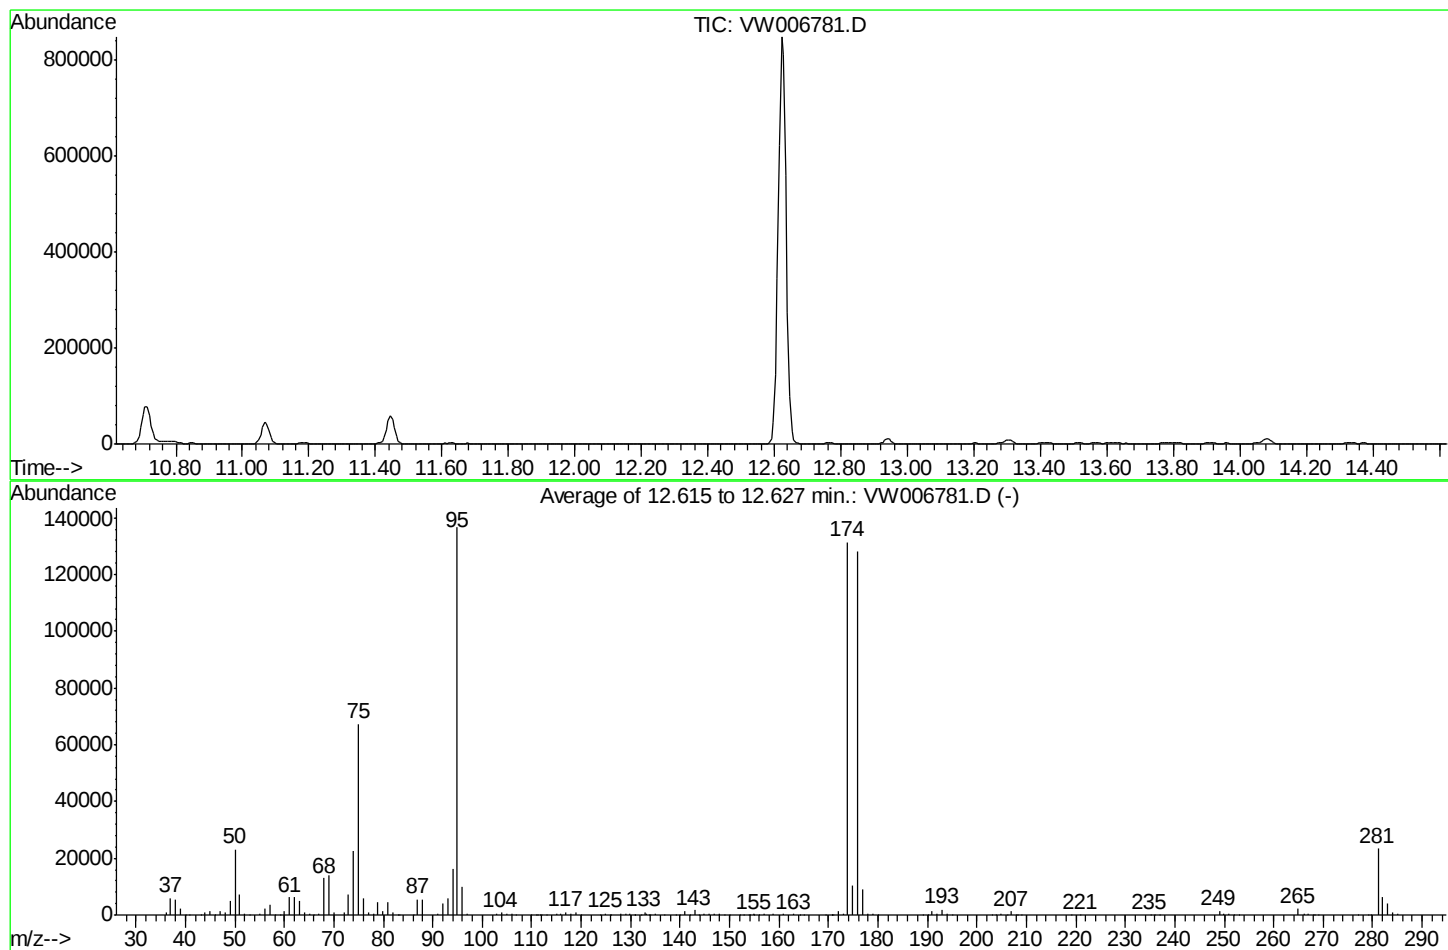

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	23034	PASS
75	95	30	60	49.3	67392	PASS
95	95	100	100	100.0	136629	PASS
96	95	5	9	7.2	9854	PASS
173	174	0.00	2	0.4	554	PASS
174	95	50	100	96.2	131480	PASS
175	174	5	9	7.8	10192	PASS
176	174	95	101	97.3	127917	PASS
177	176	5	9	7.0	8962	PASS