
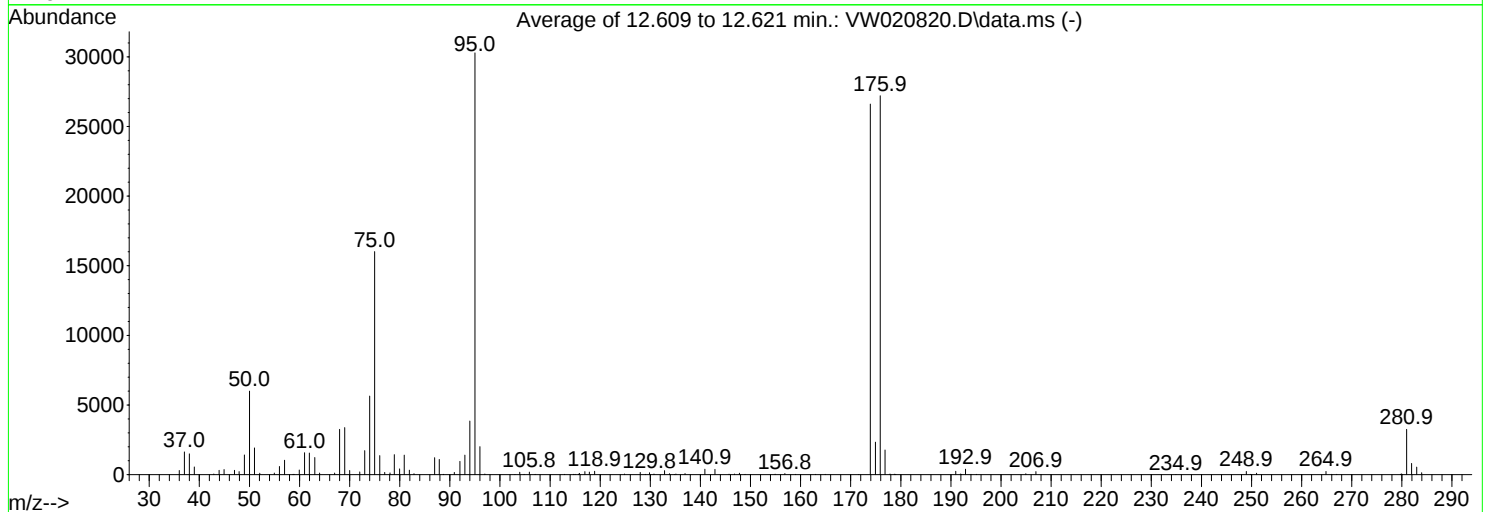


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110921\
 Data File : VW020820.D
 Acq On : 09 Nov 2021 08:10
 Operator : SY/VA
 Sample : BFB461
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB461

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Title : SFAM01.0
 Last Update : Mon Nov 15 03:01:39 2021

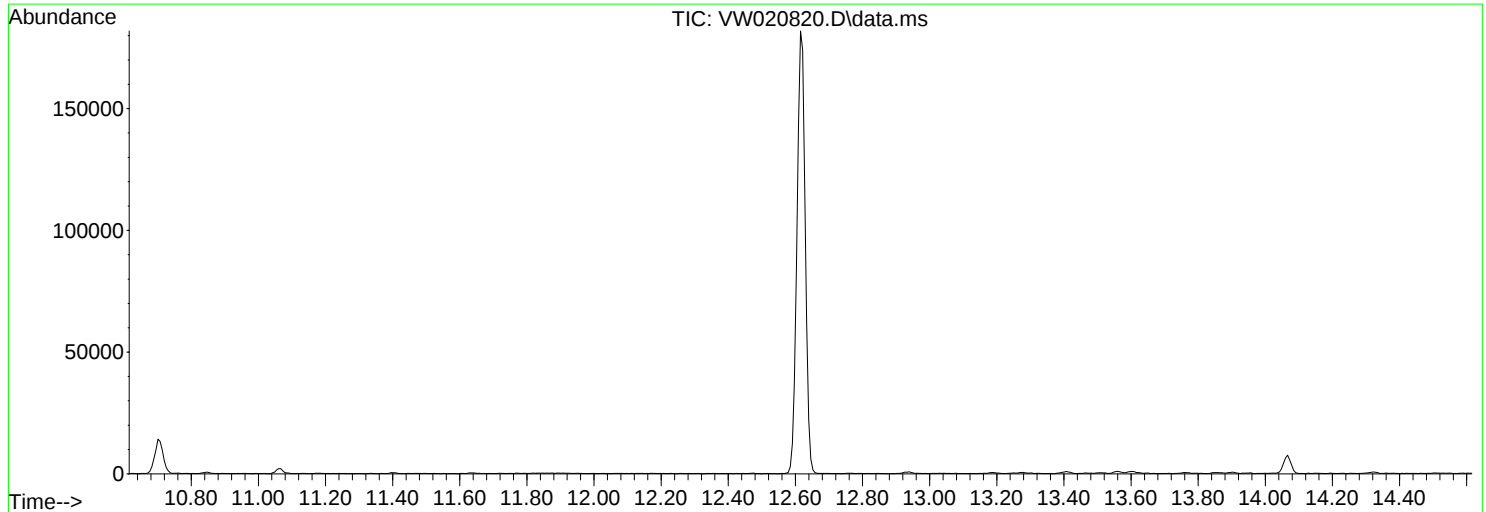

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	6000	PASS
75	95	30	80	52.9	16016	PASS
95	95	100	100	100.0	30285	PASS
96	95	5	9	6.6	2008	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.8	26605	PASS
175	174	5	9	8.8	2335	PASS
176	174	95	105	102.2	27203	PASS
177	176	5	10	6.5	1768	PASS

m/z	Abundance
39.90	73.0
44.00	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB461

m/z	Abundance
36.00	315.0
37.00	1518.0
38.00	1447.0
39.00	511.0
39.90	71.0
42.90	67.0
43.90	357.0
45.00	361.0
47.00	282.0
48.00	162.0
49.00	1149.0
50.00	5435.0
51.00	1621.0
52.00	69.0
54.90	103.0
56.00	570.0
57.00	912.0
58.70	53.0
59.90	328.0
61.00	1344.0
62.00	1440.0
63.00	1133.0
64.00	96.0
67.00	78.0
68.00	3070.0
69.00	3158.0
70.00	263.0
72.00	179.0
73.00	1695.0
74.00	4753.0
75.00	14383.0
76.00	1303.0
77.10	135.0
78.00	115.0
78.90	1198.0
79.90	318.0
80.90	1260.0
81.90	295.0
82.90	65.0
87.00	1137.0
87.90	901.0
90.90	113.0
92.00	886.0
93.00	1200.0
94.00	3402.0
95.00	25840.0
96.00	1791.0
97.00	71.0
103.00	50.0
104.00	170.0
105.90	146.0
114.70	63.0
115.70	92.0
117.00	214.0
118.00	203.0
118.90	209.0
124.90	89.0
128.00	112.0
129.90	126.0
132.90	380.0
133.90	132.0
134.80	51.0
137.00	69.0
140.80	278.0
142.90	315.0
146.80	82.0
147.80	72.0
148.90	55.0
156.90	51.0
163.00	85.0
164.90	58.0
173.90	19096.0
175.00	1695.0
175.90	20592.0
176.90	1679.0
178.70	111.0
191.00	352.0
191.90	123.0
192.90	636.0
194.00	88.0
195.10	63.0
204.90	153.0
207.00	279.0
208.00	52.0
234.90	52.0
248.90	362.0
249.80	59.0
251.00	142.0
264.90	326.0
266.00	74.0
267.00	56.0
279.70	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB461

281.00	4794.0
282.00	970.0
282.90	655.0
283.90	179.0

Instrument :
MSVOA_W
ClientSampleId :
BFB461

m/z	Abundance
35.90	323.0
37.00	1710.0
38.00	1632.0
39.00	594.0
39.90	97.0
42.90	64.0
43.90	338.0
45.00	400.0
47.10	356.0
47.90	235.0
49.00	1683.0
50.00	6676.0
51.00	2163.0
52.10	129.0
55.00	154.0
56.00	671.0
57.00	1235.0
58.90	59.0
59.90	336.0
61.00	1697.0
61.90	1749.0
63.00	1402.0
64.00	138.0
67.00	114.0
68.00	3422.0
69.00	3723.0
70.00	333.0
72.00	209.0
73.00	1840.0
74.00	6378.0
75.00	17216.0
76.00	1567.0
77.00	196.0
78.10	124.0
78.90	1641.0
80.00	499.0
80.90	1535.0
81.90	349.0
82.90	73.0
86.90	1393.0
87.90	1232.0
88.70	72.0
90.90	181.0
92.00	1043.0
93.00	1534.0
94.00	4187.0
95.00	33168.0
96.00	2289.0
97.00	73.0
104.00	164.0
105.90	222.0
115.00	56.0
115.90	141.0
116.90	228.0
117.80	161.0
118.90	276.0
124.80	61.0
128.00	168.0
129.80	120.0
130.80	73.0
132.80	310.0
133.80	67.0
135.10	74.0
136.90	96.0
140.90	423.0
142.90	426.0
145.70	60.0
146.80	63.0
147.80	115.0
156.80	81.0
159.00	56.0
173.90	29272.0
174.90	2591.0
175.90	30072.0
176.80	1875.0
177.90	87.0
179.00	85.0
191.00	216.0
192.10	83.0
192.90	392.0
205.00	58.0
206.90	238.0
249.00	212.0
251.00	90.0
264.80	213.0
279.90	160.0
280.90	2981.0
281.90	874.0
283.00	548.0
284.00	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB461

m/z	Abundance
36.10	266.0
37.00	1667.0
38.00	1413.0
39.00	564.0
44.00	433.0
44.90	331.0
46.90	303.0
48.00	252.0
49.00	1424.0
50.00	5890.0
51.00	1977.0
52.10	105.0
55.00	87.0
56.00	531.0
57.00	948.0
60.00	339.0
61.00	1678.0
62.00	1465.0
63.10	1151.0
64.00	107.0
67.00	160.0
68.00	3272.0
69.00	3243.0
70.00	309.0
72.00	192.0
73.00	1639.0
74.00	5795.0
75.00	16448.0
76.00	1241.0
76.90	146.0
78.10	134.0
78.90	1475.0
80.00	432.0
80.90	1397.0
81.90	318.0
82.80	53.0
86.90	1130.0
87.90	1157.0
90.90	183.0
92.00	946.0
93.00	1483.0
94.00	3966.0
95.00	31848.0
96.00	1945.0
103.90	182.0
104.80	55.0
105.80	169.0
107.00	53.0
112.90	53.0
115.80	139.0
116.90	206.0
117.80	189.0
118.90	246.0
128.00	188.0
129.00	67.0
129.90	154.0
130.70	55.0
132.90	178.0
135.10	69.0
136.90	74.0
141.00	471.0
142.90	401.0
145.70	55.0
147.80	111.0
154.90	104.0
156.90	103.0
171.60	52.0
173.90	31448.0
174.90	2718.0
175.90	30944.0
176.90	1750.0
177.80	60.0
190.80	156.0
193.00	159.0
207.00	137.0
248.90	122.0
250.90	65.0
264.80	165.0
280.10	79.0
281.00	1985.0
282.00	581.0
283.00	401.0
283.90	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB461