



Trichlorofluoromethane

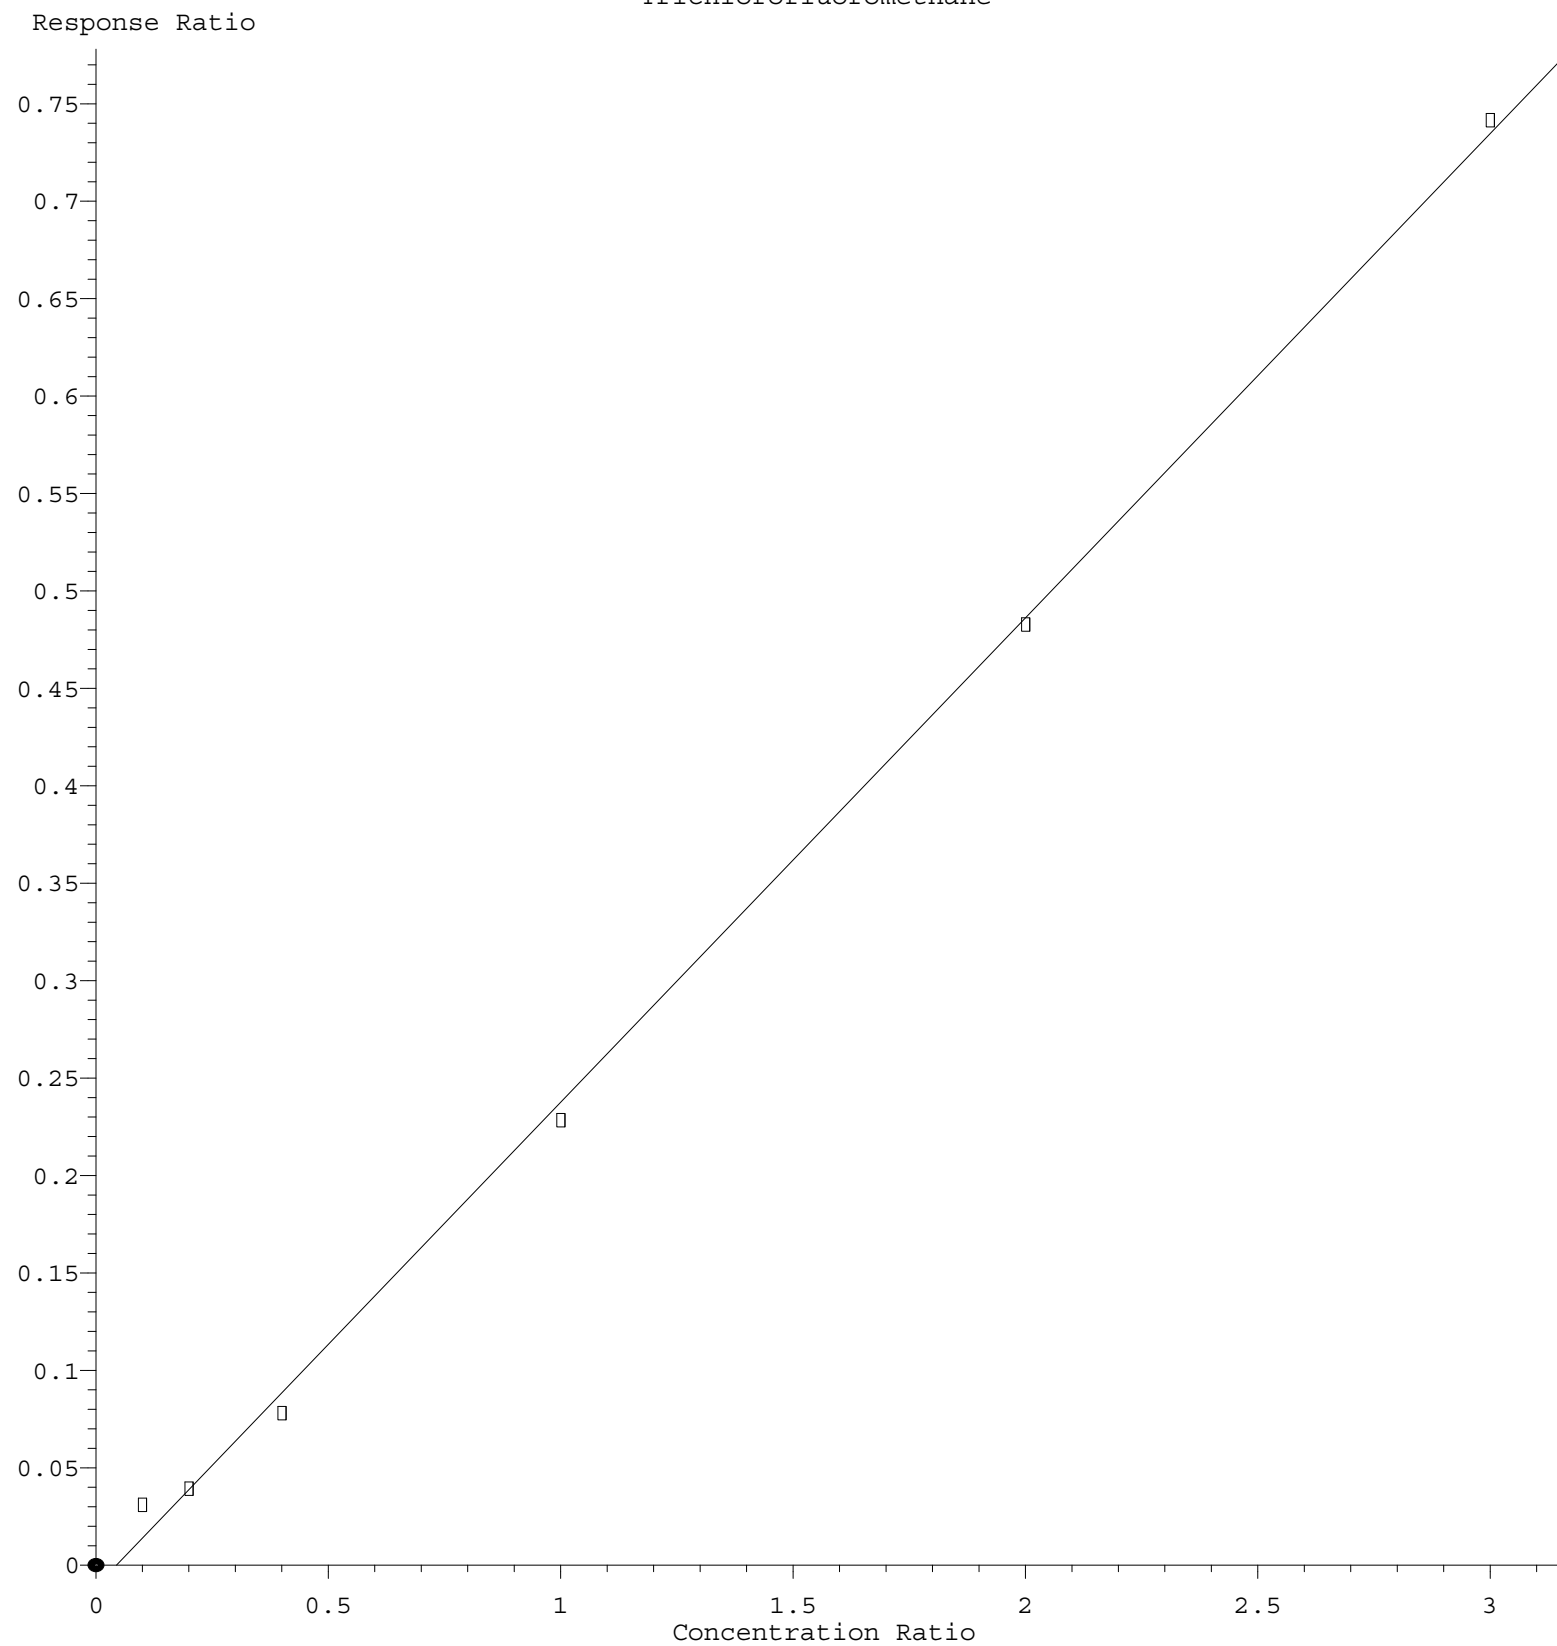

Response = 2.487e-001 * Amt - 1.086e-002
 Coef of Det (r^2) = 0.998694 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111021S.M
 Calibration Table Last Updated: Sat Nov 13 07:30:48 2021


Bromomethane

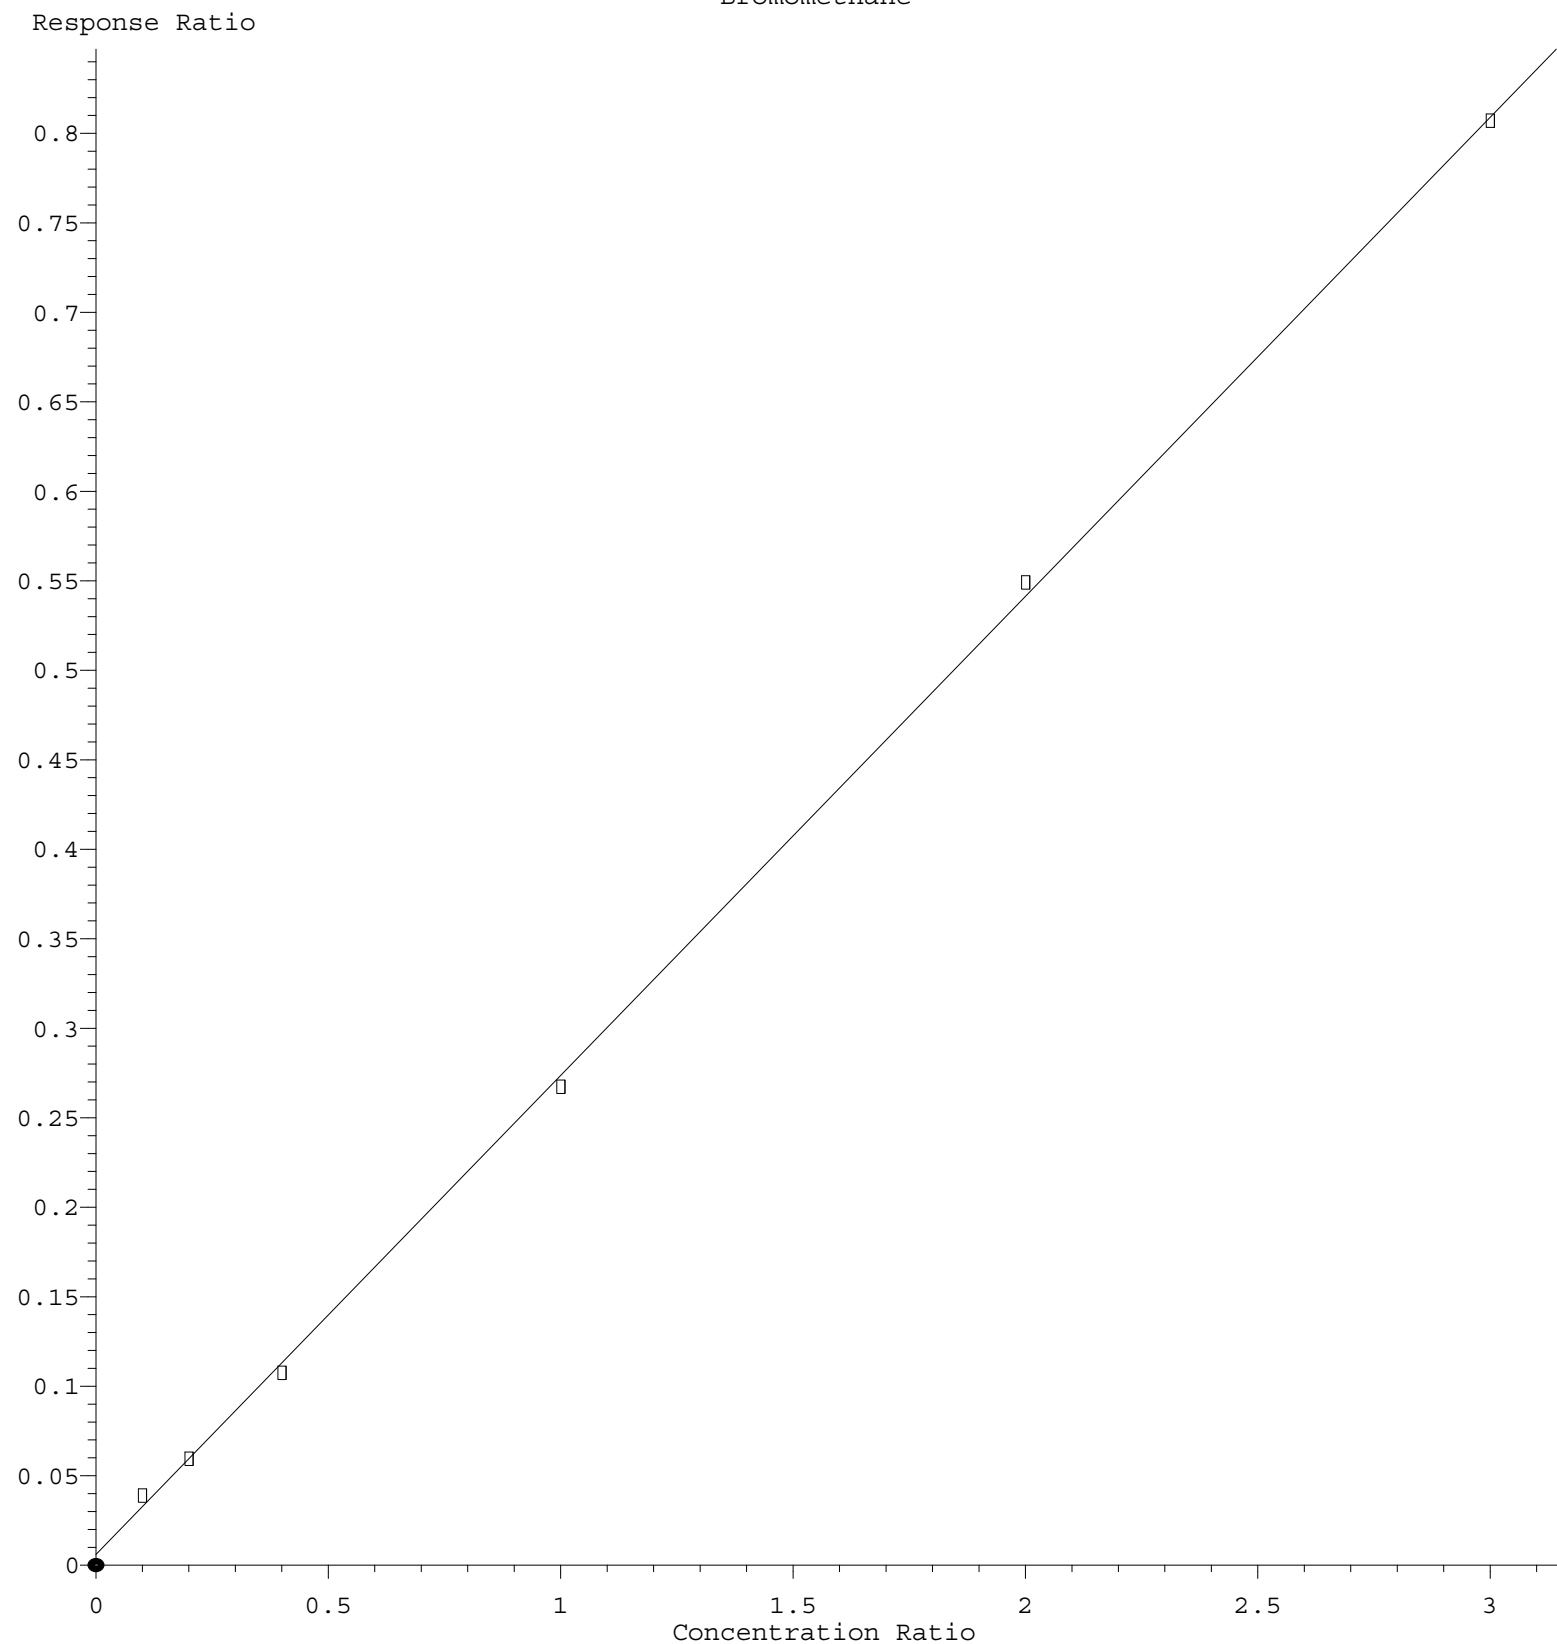

Response = 2.679e-001 * Amt + 5.670e-003
 Coef of Det (r^2) = 0.999644 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111021S.M
 Calibration Table Last Updated: Sat Nov 13 07:30:48 2021

Acetone


Response Ratio

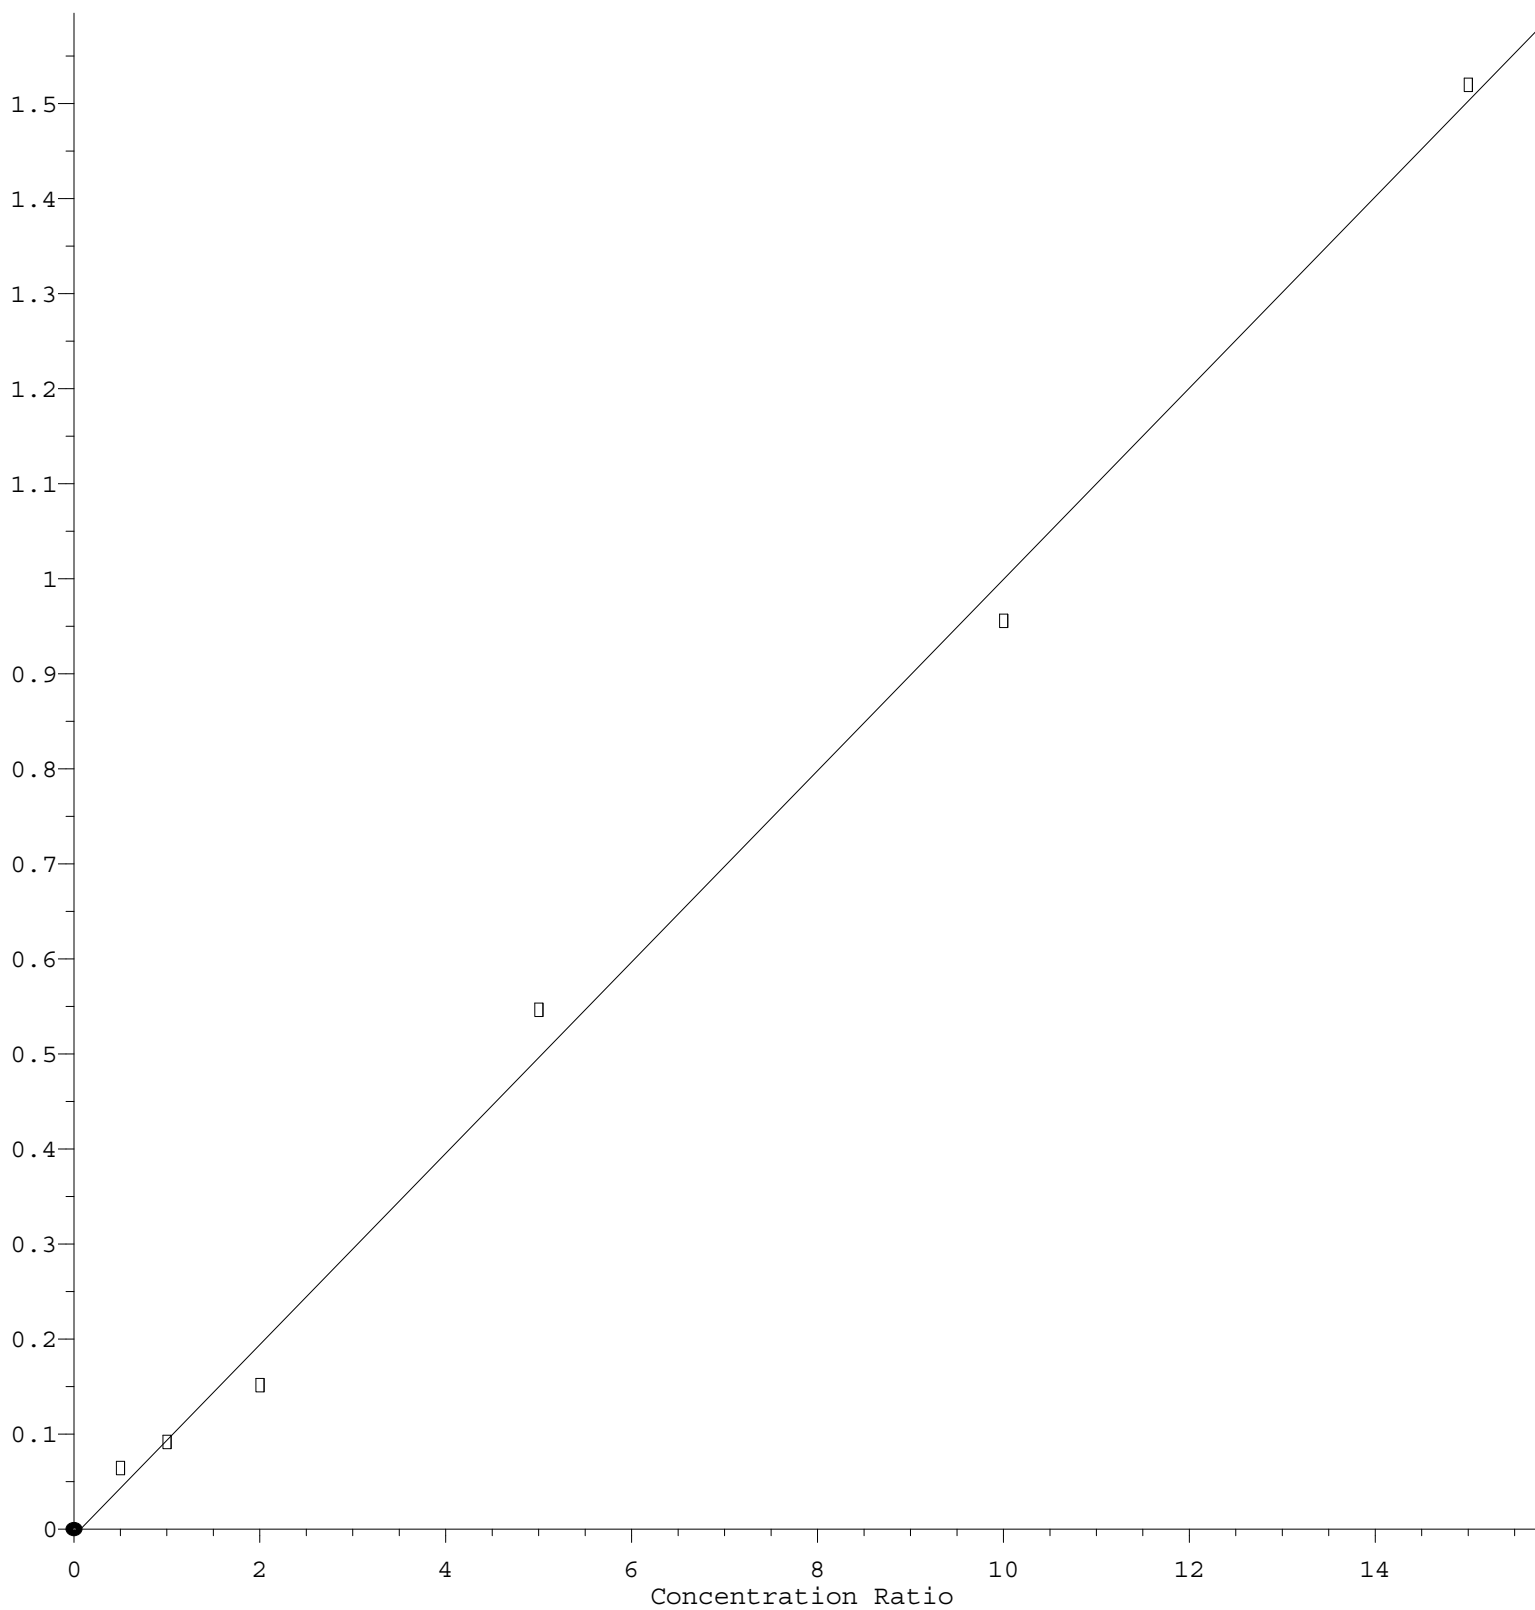

$\text{Response} = 1.006\text{e-}001 * \text{Amt} - 6.801\text{e-}003$
 Coef of Det (r^2) = 0.995910 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111021S.M
 Calibration Table Last Updated: Sat Nov 13 07:30:48 2021

Methylene Chloride

Response Ratio

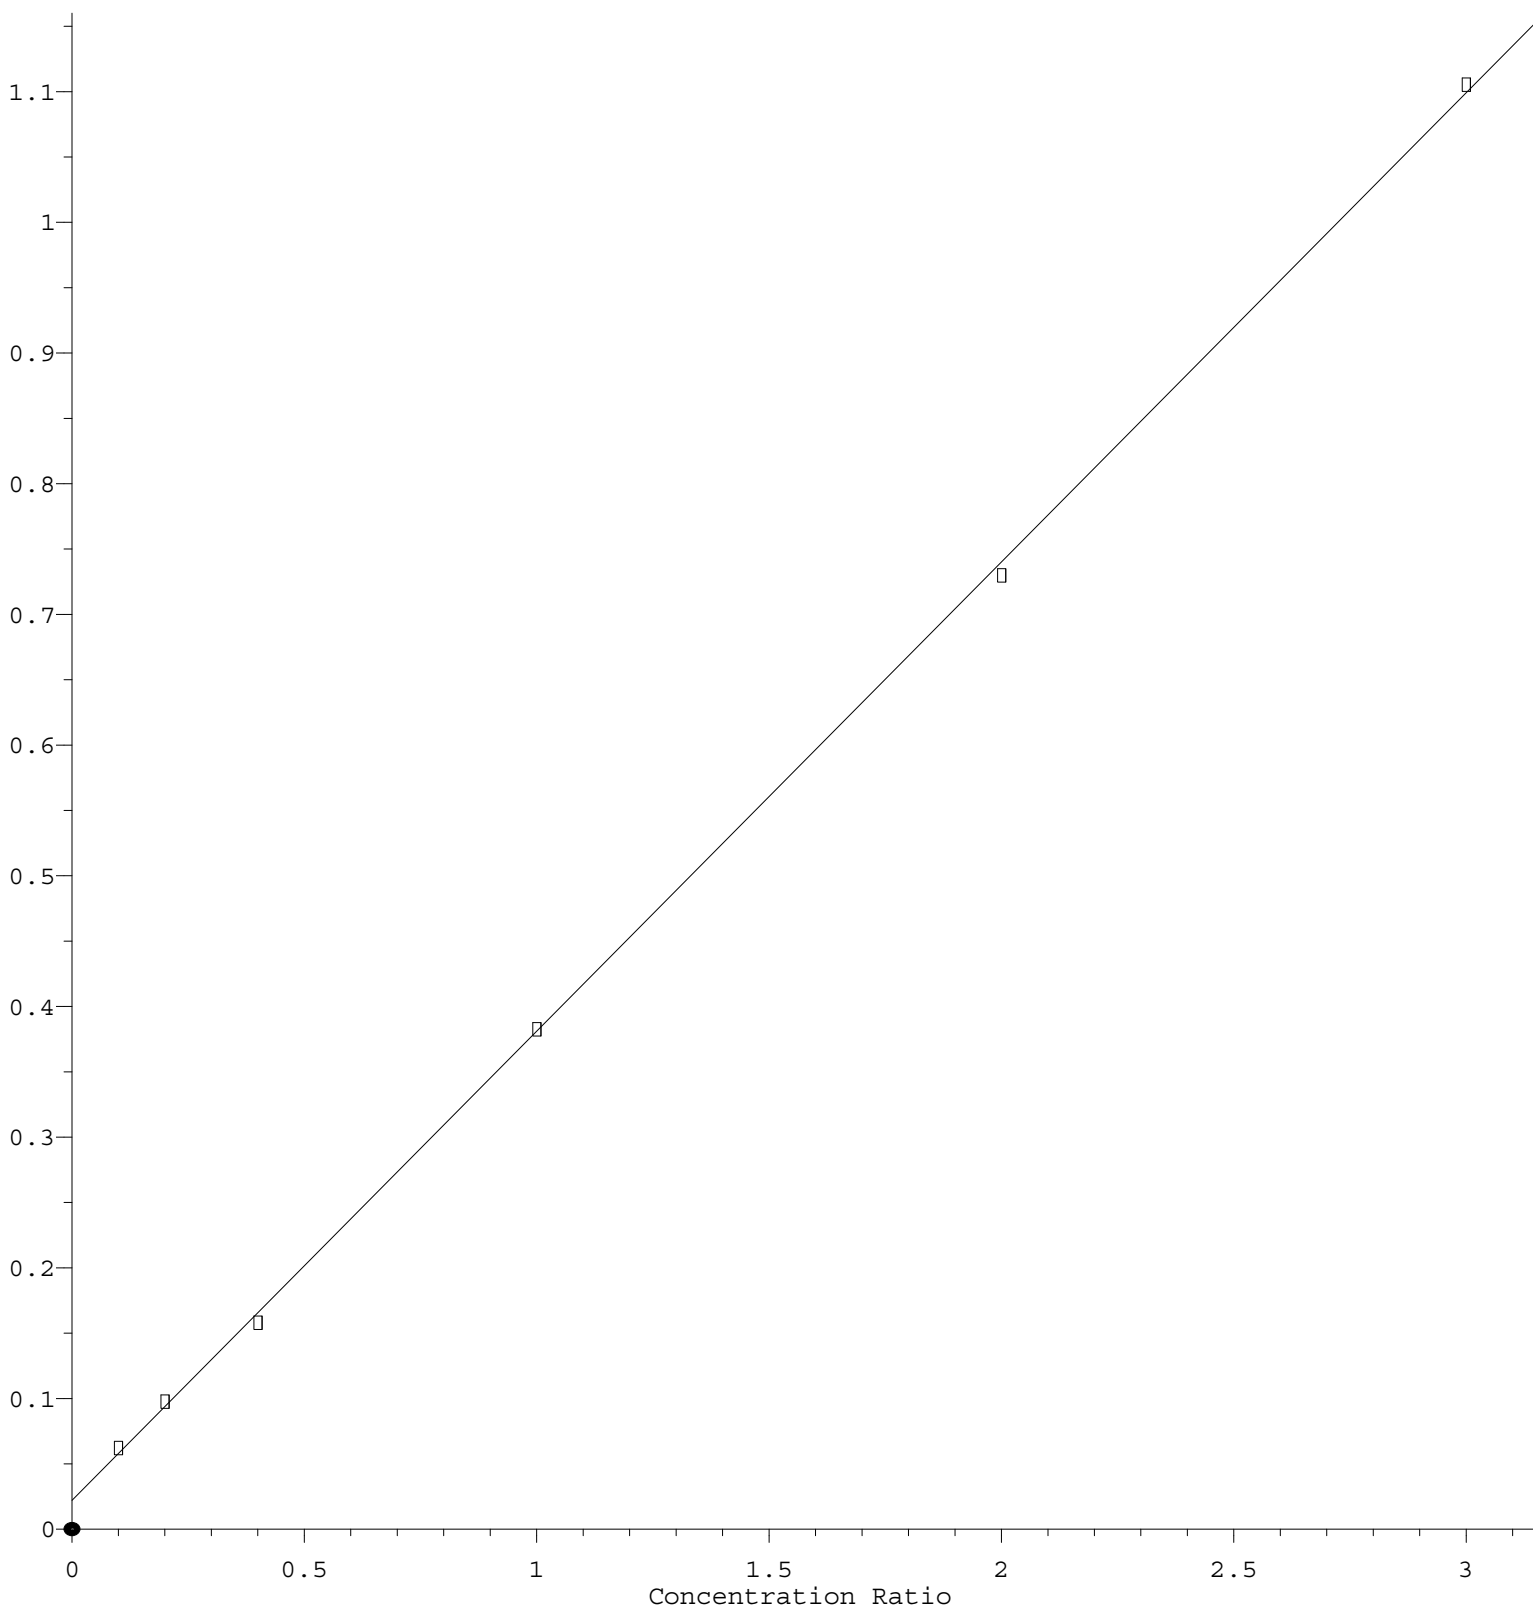

$$\text{Response} = 3.591\text{e-}001 * \text{Amt} + 2.155\text{e-}002$$

Coef of Det (r^2) = 0.999729 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111021S.M

Calibration Table Last Updated: Sat Nov 13 07:30:48 2021