
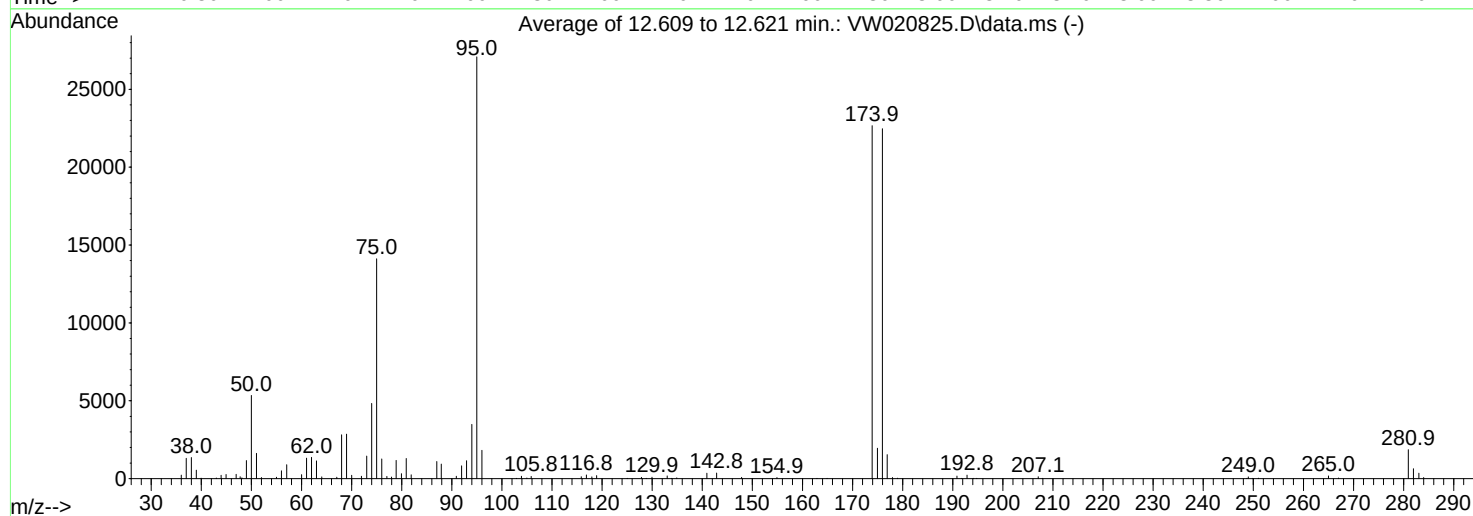


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111021\
 Data File : VW020825.D
 Acq On : 10 Nov 2021 09:50
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111021S.M
 Title : SW846 8260
 Last Update : Sat Nov 13 07:30:48 2021

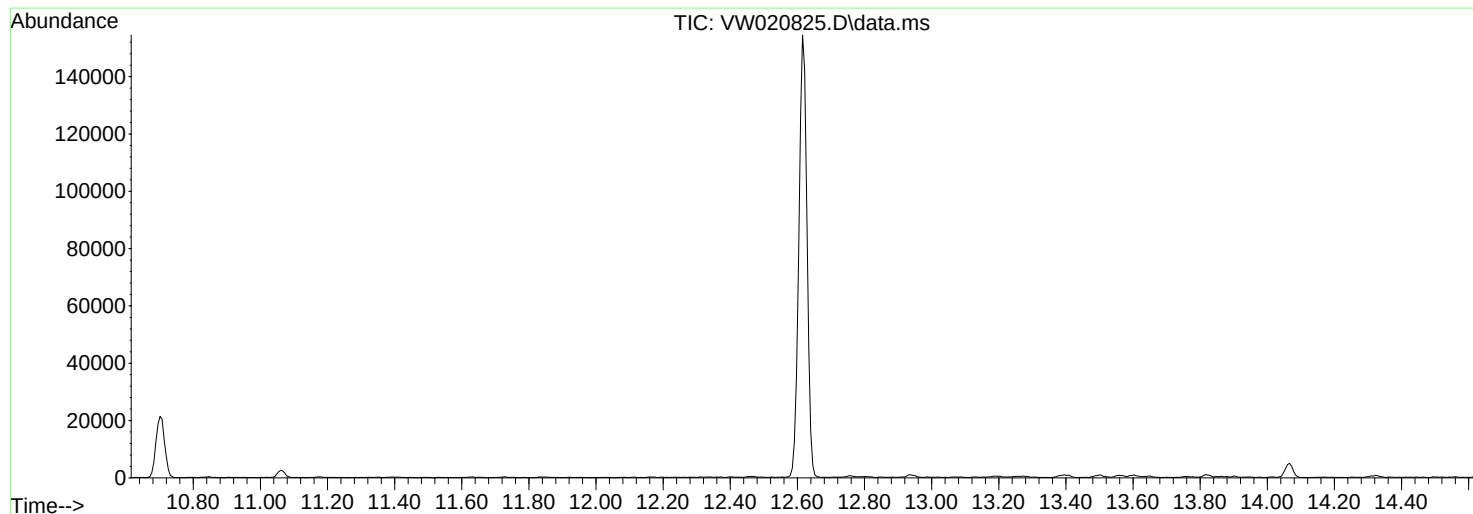

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	5339	PASS
75	95	30	60	52.1	14122	PASS
95	95	100	100	100.0	27085	PASS
96	95	5	9	6.7	1817	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.7	22669	PASS
175	174	5	9	8.6	1950	PASS
176	174	95	101	99.1	22469	PASS
177	176	5	9	6.9	1540	PASS