

Data File : VW013962.D
Acq On : 11 Nov 2019 16:00
Operator : SY/VA
Sample : VW1111SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK22

Quant Time: Nov 12 06:13:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 06:10:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	333332	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	323071	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	184050	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	115593	21.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.96%
7) Chloroethane-d5	2.88	69	88649	20.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.24%
10) 1,1-Dichloroethene-d2	4.01	63	170914	15.66	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.64%
20) 2-Butanone-d5	7.07	46	71690	46.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.80%
24) Chloroform-d	7.64	84	208892	20.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.52%
26) 1,2-Dichloroethane-d4	8.30	65	113128	21.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.80%
29) Benzene-d6	8.27	84	467366	20.39	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.56%
33) 1,2-Dichloropropane-d6	9.27	67	137378	20.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.84%
37) Toluene-d8	10.32	98	440041	20.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.96%
38) trans-1,3-Dichloropropene-	10.58	79	61784	21.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.92%
39) 2-Hexanone-d5	10.92	63	59050	46.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	111625	22.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.04%
61) 1,2-Dichlorobenzene-d4	13.85	152	151844	20.53	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.12%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.55	75	18887	5.132 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW013962.D
Acq On : 11 Nov 2019 16:00
Operator : SY/VA
Sample : VW1111SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK22

Quant Time: Nov 12 06:13:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 06:10:10 2019
Response via : Initial Calibration

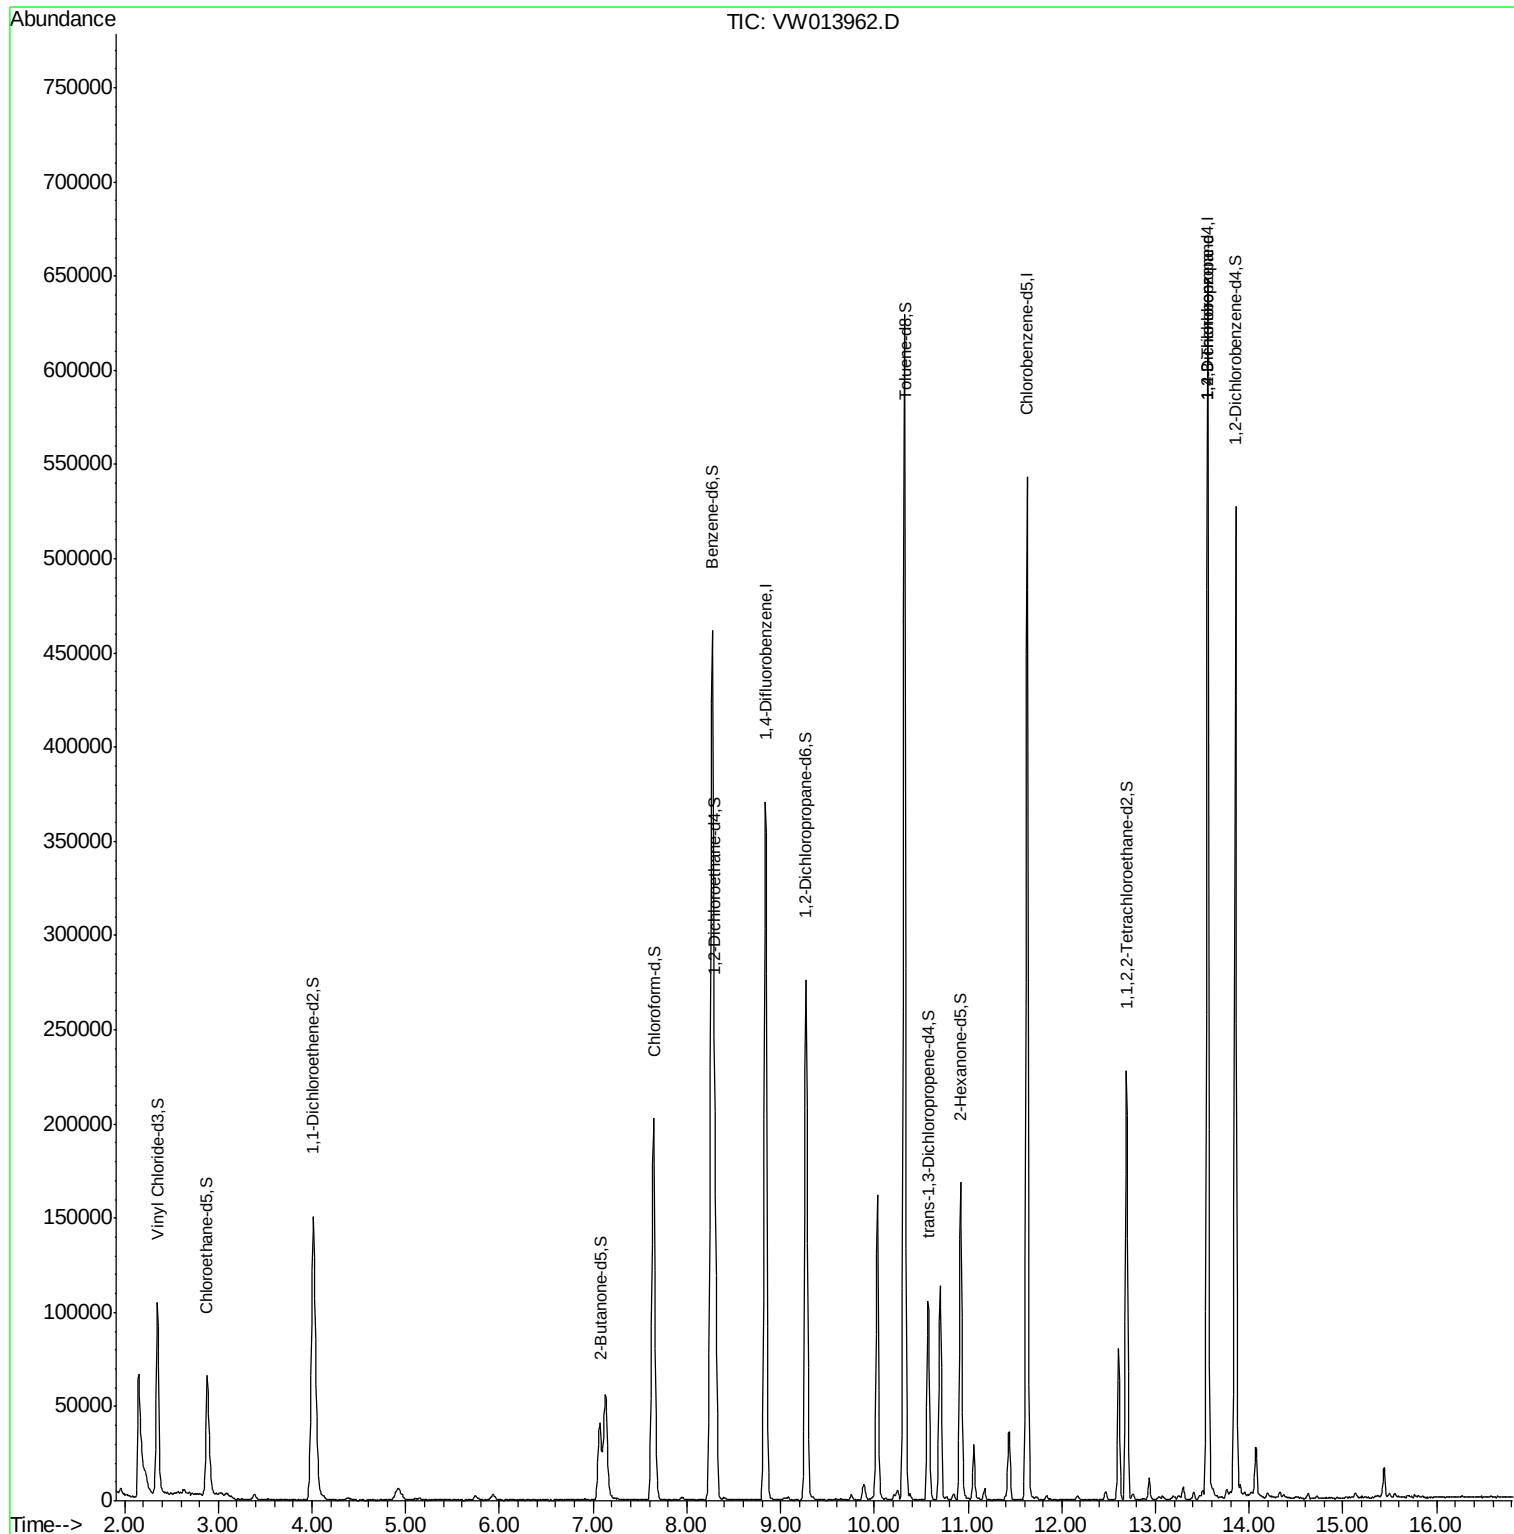

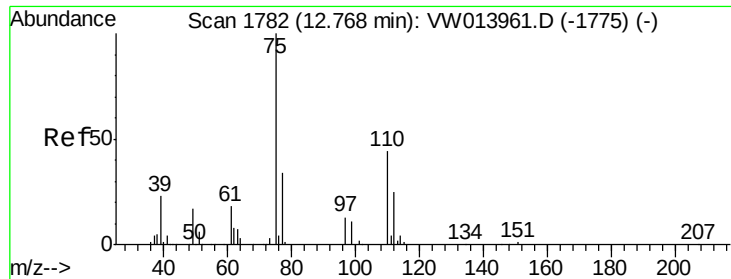

#59

1,2,3-Trichloropropane

Concen: 5.132 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013962.D

Acq: 11 Nov 2019 16:00

Instrument :

MSVOA_W

ClientSampleId :

VBLK22

Tgt Ion: 75 Resp: 18887

Ion Ratio Lower Upper

75 100

77 35.4 25.9 38.9

