

Data File : VW013970.D
Acq On : 11 Nov 2019 20:11
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK02

Quant Time: Nov 12 06:14:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 06:10:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	303744	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	300619	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	176140	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	114078	23.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.16%
7) Chloroethane-d5	2.89	69	86656	22.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.24%
10) 1,1-Dichloroethene-d2	4.02	63	166080	16.70	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.80%
20) 2-Butanone-d5	7.07	46	78187	55.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.08%
24) Chloroform-d	7.65	84	221312	23.70	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	8.40	65	100	0.02	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.08%#
29) Benzene-d6	8.27	84	484085	22.70	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.80%
33) 1,2-Dichloropropane-d6	9.27	67	145109	23.22	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.88%
37) Toluene-d8	10.32	98	458346	22.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.64%
38) trans-1,3-Dichloropropene-	10.57	79	64227	24.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.00%
39) 2-Hexanone-d5	10.92	63	66551	56.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	123843	26.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	170536	24.10	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.40%


Target Compounds					Qvalue
49) 2-Hexanone	10.92	43	7236	2.864 ug/L #	68
59) 1,2,3-Trichloropropane	13.55	75	17689	5.165 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW013970.D
Acq On : 11 Nov 2019 20:11
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK02

Quant Time: Nov 12 06:14:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 06:10:10 2019
Response via : Initial Calibration




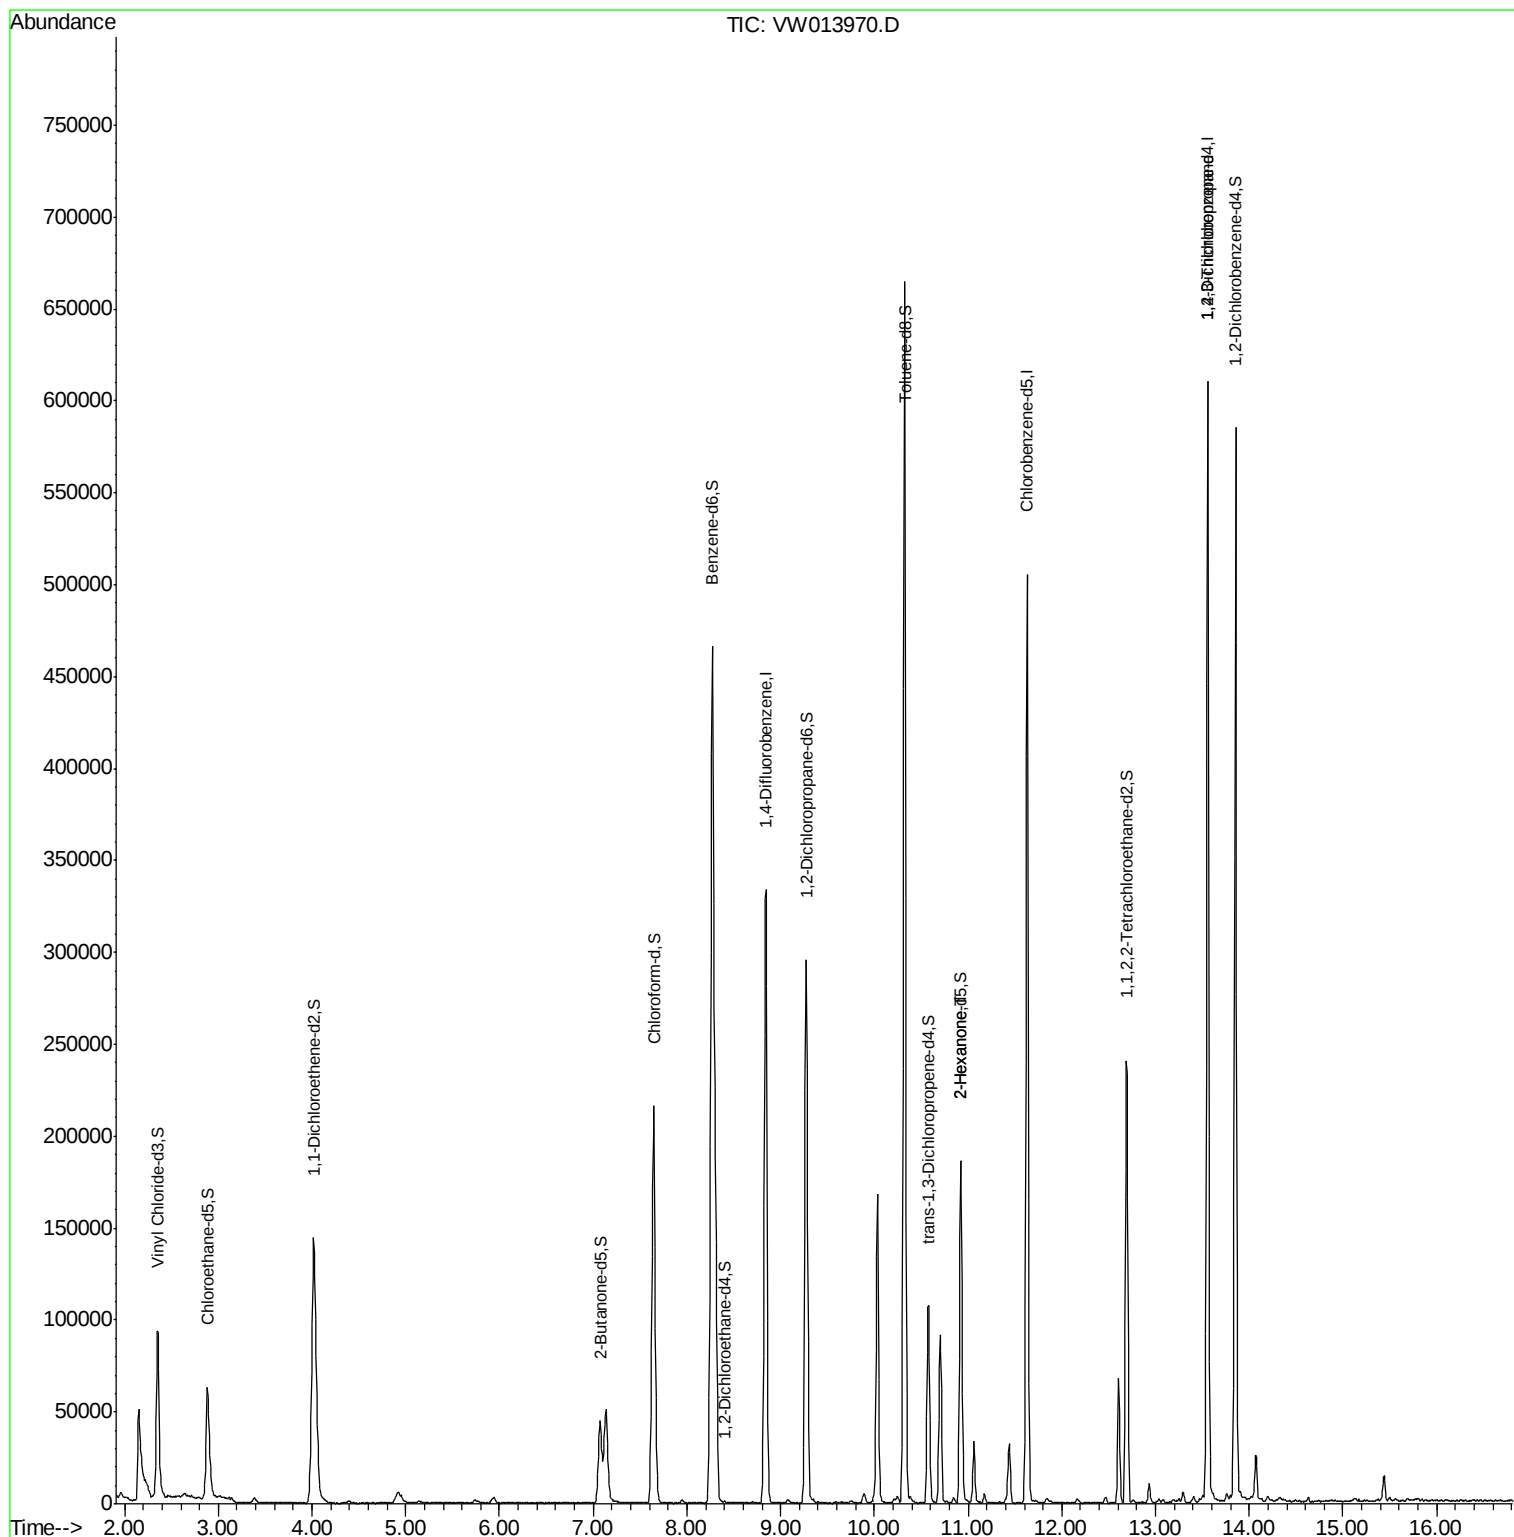


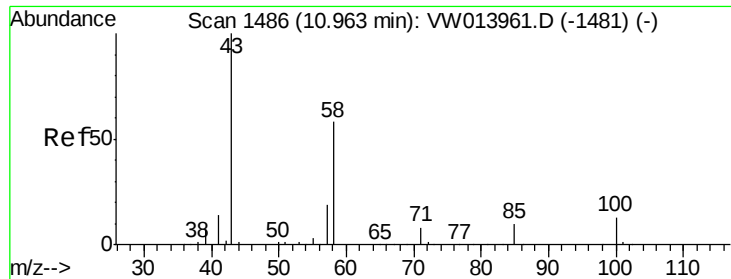

#49
2-Hexanone
Concen: 2.864 ug/L
RT: 10.92 min Scan# 1479
Delta R.T. -0.04 min
Lab File: VW013970.D
Acq: 11 Nov 2019 20:11

Instrument :
MSVOA_W
ClientSampleId :
VIBLK02

Tgt Ion: 43 Resp: 7236
Ion Ratio Lower Upper
43 100
58 27.6 44.4 66.6#
57 27.4 16.5 24.7#
100 0.0 11.1 16.7#

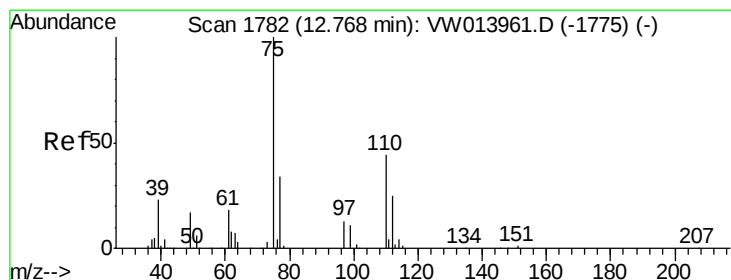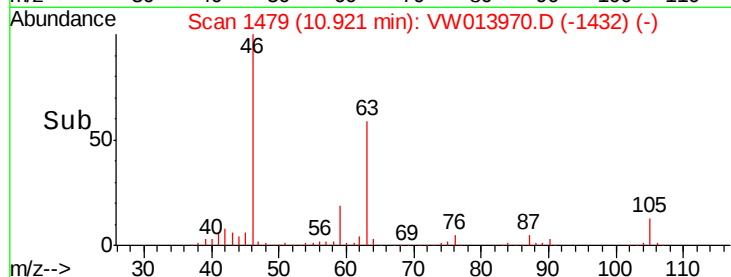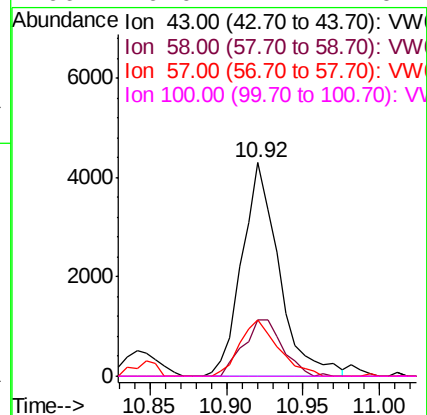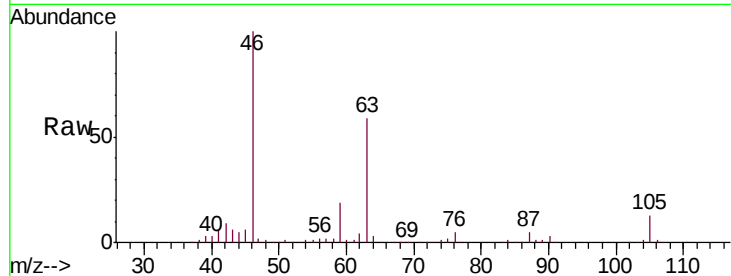

#59
1,2,3-Trichloropropane
Concen: 5.165 ug/L
RT: 13.55 min Scan# 1911
Delta R.T. 0.79 min
Lab File: VW013970.D
Acq: 11 Nov 2019 20:11

Tgt Ion: 75 Resp: 17689
Ion Ratio Lower Upper
75 100
77 37.3 25.9 38.9

