


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111218\
Data File : VW006820.D
Acq On : 12 Nov 2018 21:37
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111218S.M
Title : SW846 8260
Last Update : Mon Nov 12 14:58:58 2018

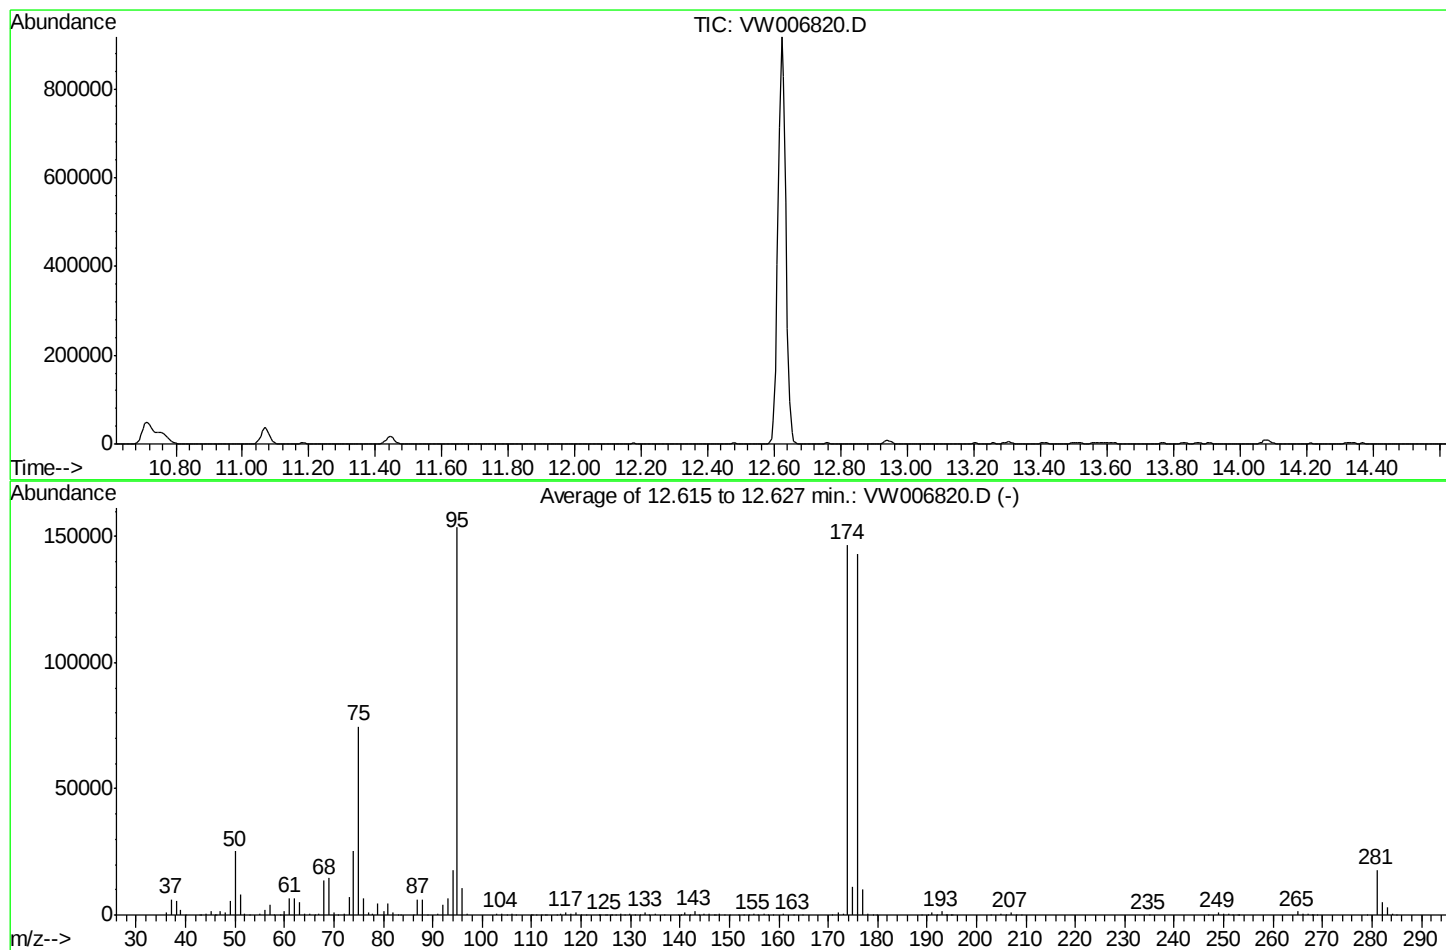

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	25154	PASS
75	95	30	60	48.6	74744	PASS
95	95	100	100	100.0	153664	PASS
96	95	5	9	6.9	10528	PASS
173	174	0.00	2	0.4	639	PASS
174	95	50	100	95.5	146770	PASS
175	174	5	9	7.6	11096	PASS
176	174	95	101	97.4	142922	PASS
177	176	5	9	6.9	9917	PASS