


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111318\
Data File : VW006846.D
Acq On : 13 Nov 2018 10:49
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111218S.M
Title : SW846 8260
Last Update : Mon Nov 12 14:58:58 2018

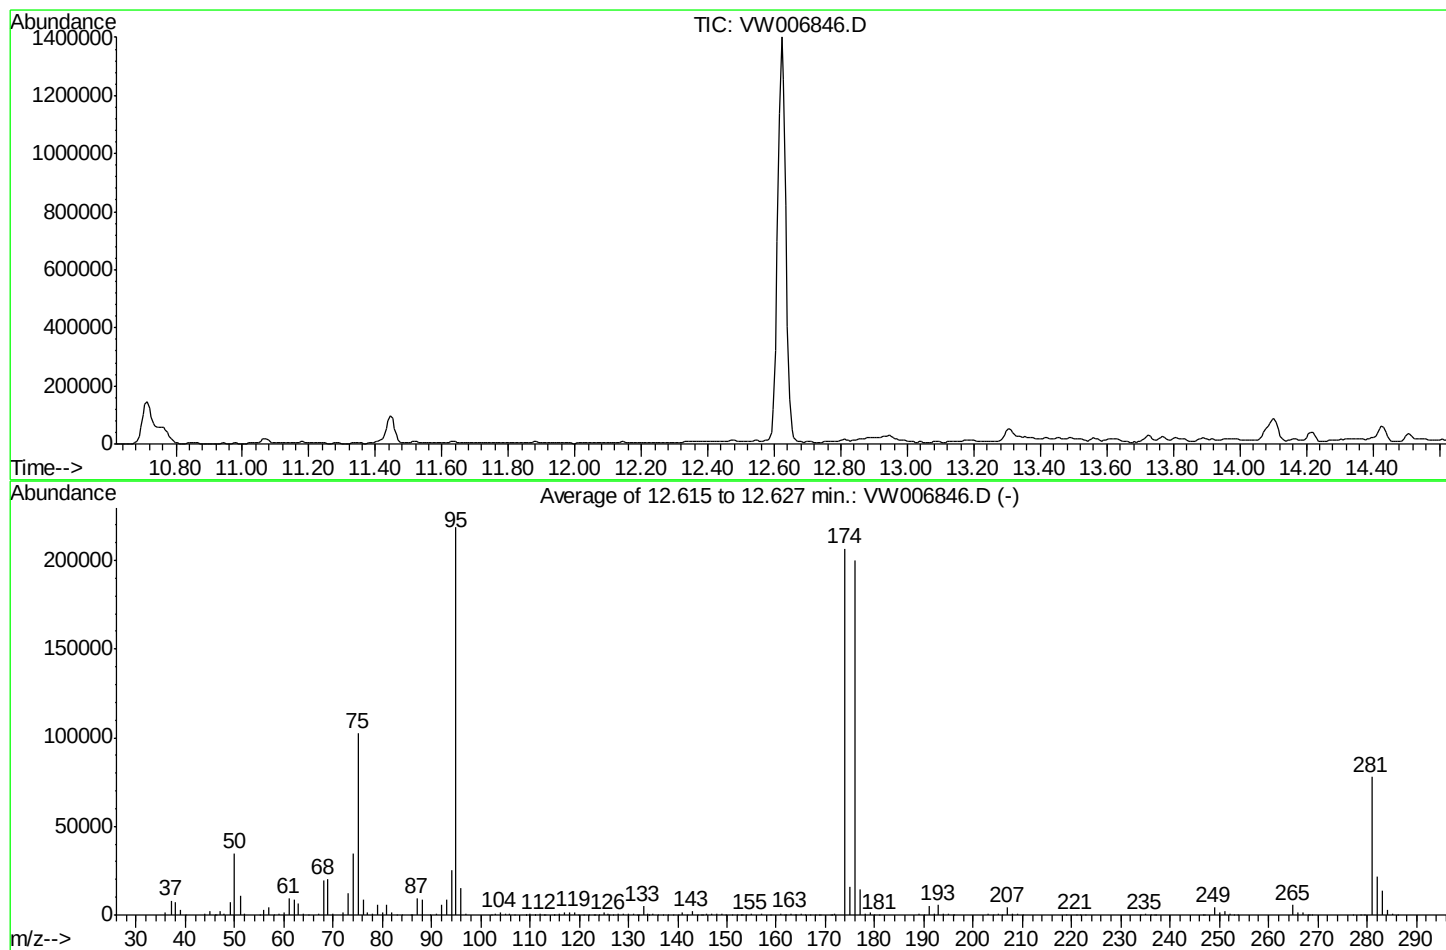

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	34440	PASS
75	95	30	60	46.8	102432	PASS
95	95	100	100	100.0	218640	PASS
96	95	5	9	7.0	15312	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.6	206762	PASS
175	174	5	9	7.5	15600	PASS
176	174	95	101	96.6	199680	PASS
177	176	5	9	7.4	14785	PASS