

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
Data File : VW017206.D
Acq On : 13 Nov 2020 12:42
Operator : SY/VA
Sample : L4711-04
Misc : 5.49G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AZ8

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:51:15 PM

Quant Time: Nov 16 14:15:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

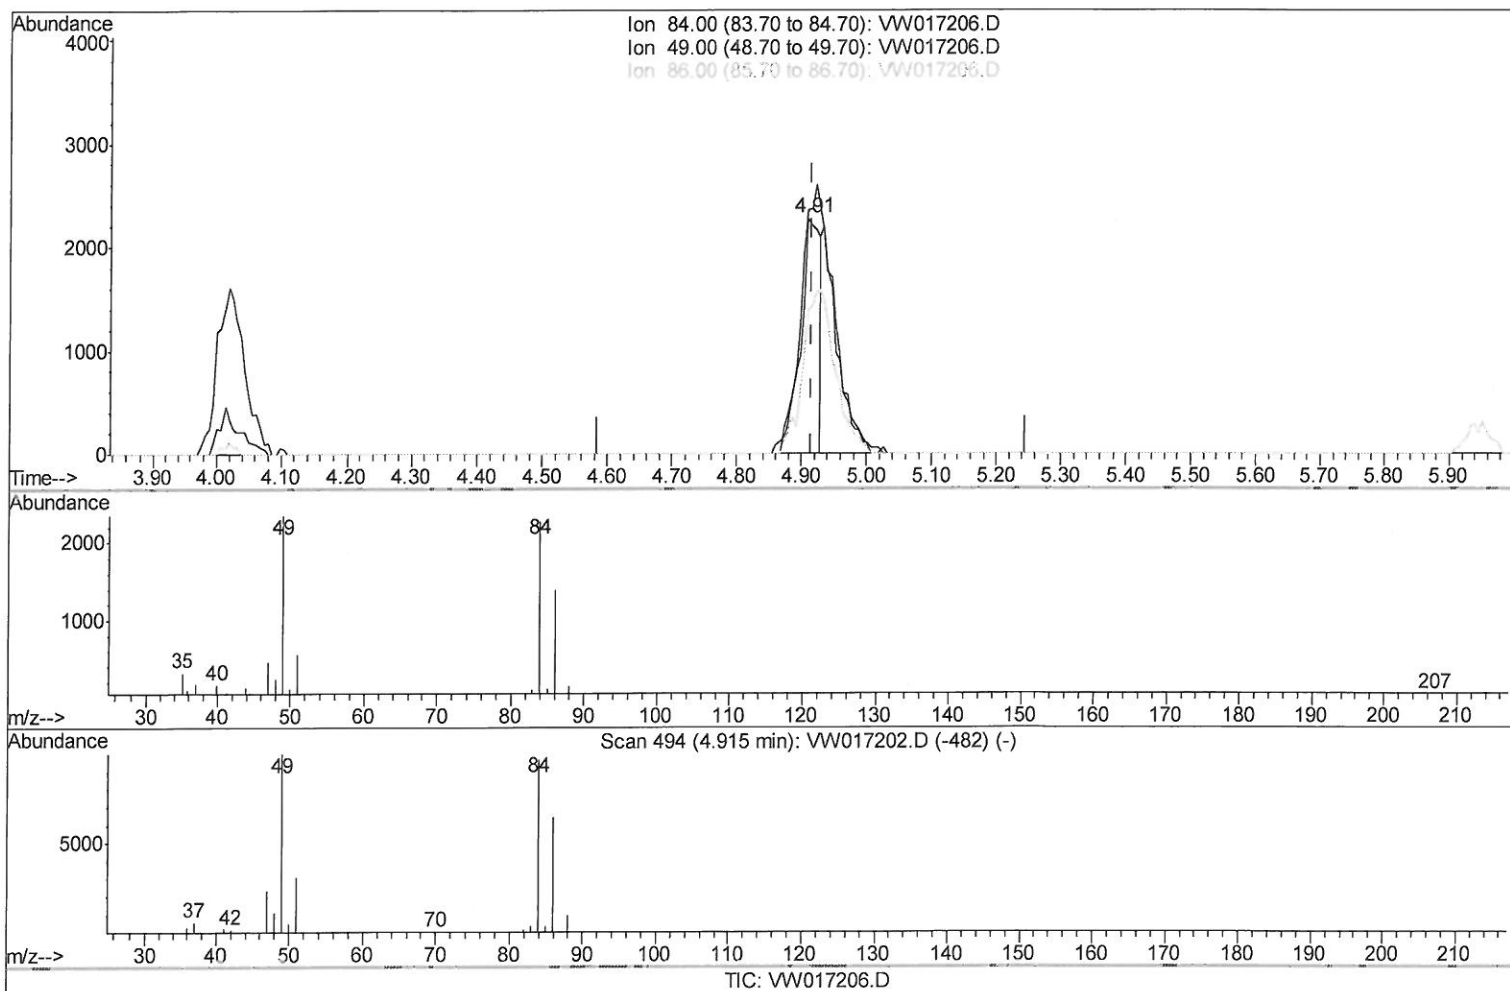

(16) Methylene chloride (T)

4.909min (-0.006) 0.81ug/L

response 4763

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	103.38
86.00	64.40	60.97
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
Data File : VW017206.D
Acq On : 13 Nov 2020 12:42
Operator : SY/VA
Sample : L4711-04
Misc : 5.49G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AZ8

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:51:15 PM

Quant Time: Nov 16 14:15:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

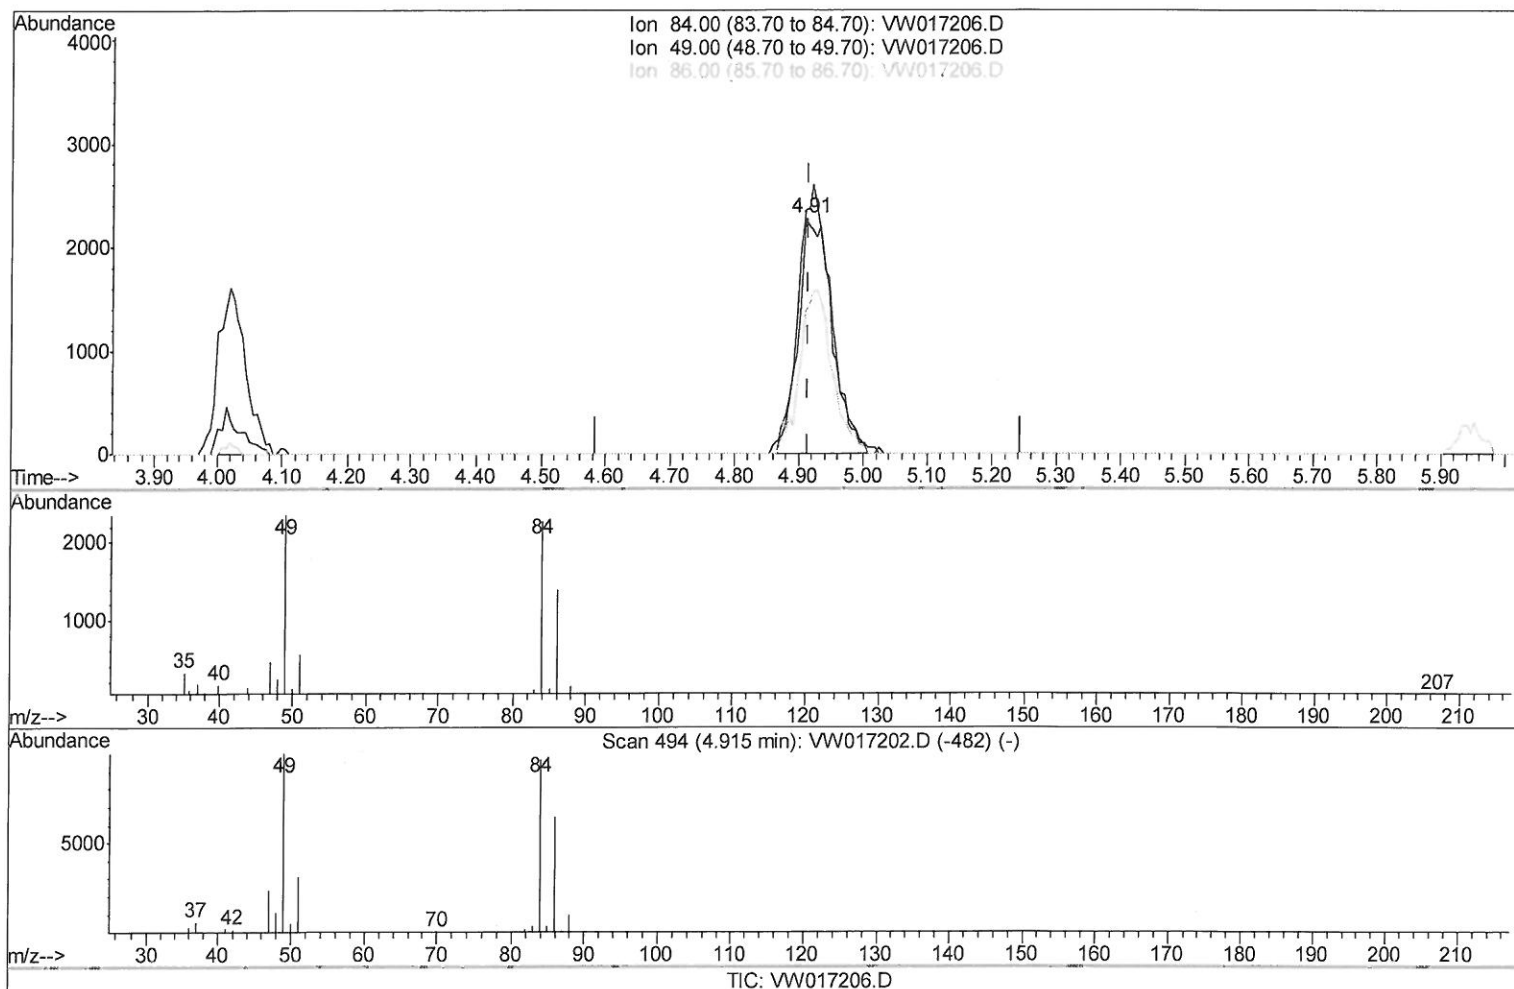

(16) Methylene chloride (T)

4.909min (-0.006) 1.41ug/L m

response 8297

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	103.38
86.00	64.40	60.97
0.00	0.00	0.00

> 11/18/20 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
 Data File : VW017206.D
 Acq On : 13 Nov 2020 12:42
 Operator : SY/VA
 Sample : L4711-04
 Misc : 5.49G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AZ8

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:51:15 PM

Quant Time: Nov 17 04:26:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	437097	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	369049	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	143389	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	102262	18.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.28%
7) Chloroethane-d5	2.89	69	87349	20.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.36%
10) 1,1-Dichloroethene-d2	4.02	63	151455	15.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.52%
20) 2-Butanone-d5	7.09	46	38666	31.41	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.82%
24) Chloroform-d	7.65	84	215058	21.08	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.32%
26) 1,2-Dichloroethane-d4	8.31	65	110240	21.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.92%
29) Benzene-d6	8.27	84	424153	22.57	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.28%
33) 1,2-Dichloropropane-d6	9.28	67	115078	22.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.56%
37) Toluene-d8	10.33	98	390741	22.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.20%
38) trans-1,3-Dichloropropene-	10.58	79	45238	19.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.20%
39) 2-Hexanone-d5	10.93	63	31125	34.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82889	18.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	109787	21.73	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.92%

Target Compounds

					Ovalue
13) Acetone	4.14	43	2182	2.647 ug/L	68
16) Methylene chloride	4.91	84	8297m	1.408 ug/L	94
43) 4-Methyl-2-pentanone	10.22	43	2096	0.750 ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
Data File : VW017206.D
Acq On : 13 Nov 2020 12:42
Operator : SY/VA
Sample : L4711-04
Misc : 5.49G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0AZ8

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:51:15 PM

Quant Time: Nov 17 04:26:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

