

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
 Data File : VW017223.D
 Acq On : 13 Nov 2020 19:20
 Operator : SY/VA
 Sample : L4710-08
 Misc : 4.93G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 C0AX7

Manual Integrations
APPROVED

MMDadoda
 11/17/2020 6:51:27 PM

Quant Time: Nov 16 14:17:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

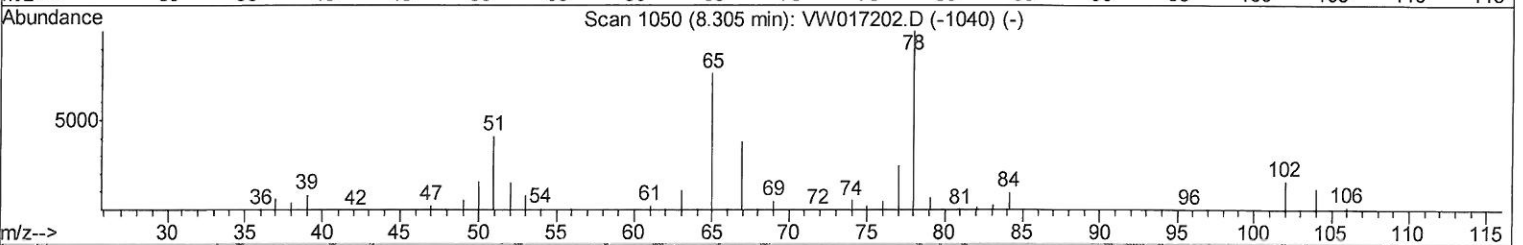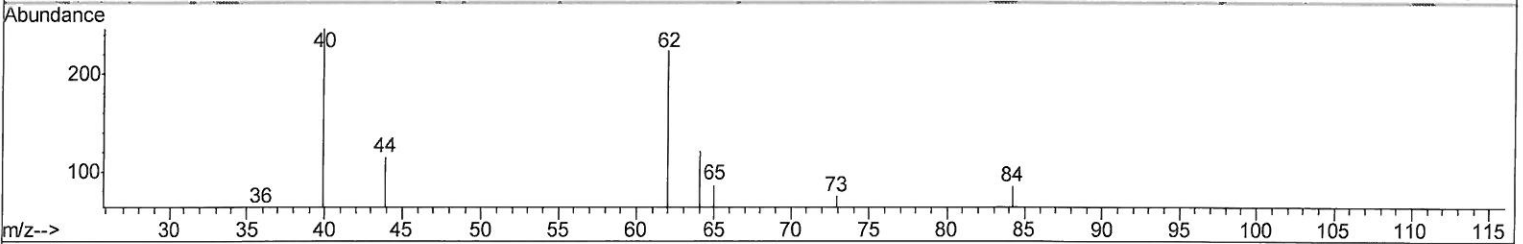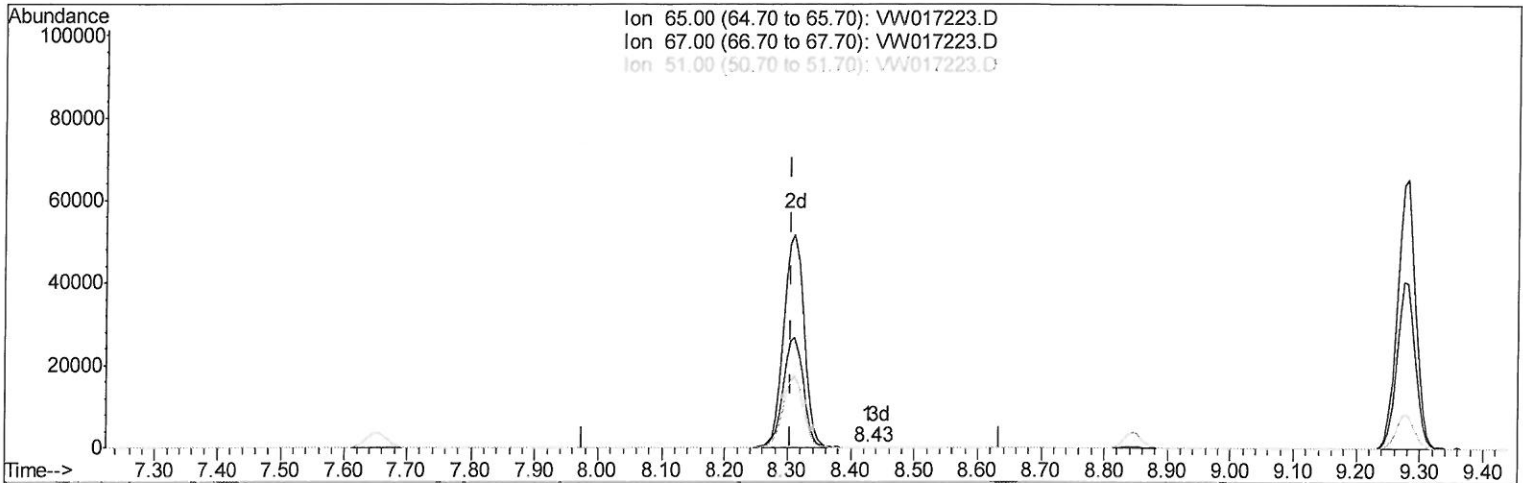

TIC: VW017223.D

(26) 1,2-Dichloroethane-d4 (S)

8.427min (+0.122) 0.02ug/L

response 87

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	65.52
51.00	92.10	73.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
 Data File : VW017223.D
 Acq On : 13 Nov 2020 19:20
 Operator : SY/VA
 Sample : L4710-08
 Misc : 4.93G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AX7

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:51:27 PM

Quant Time: Nov 16 14:17:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

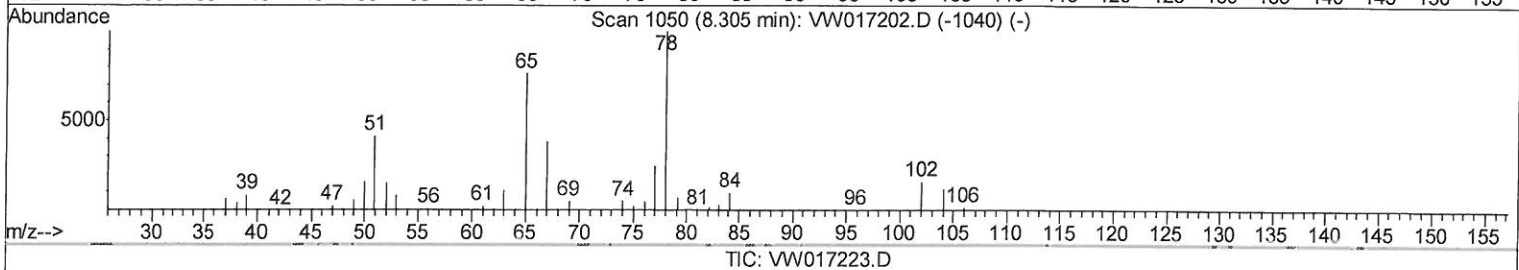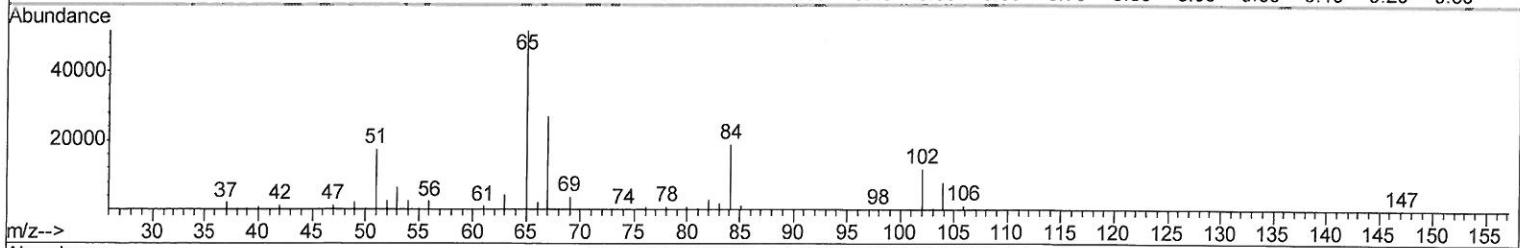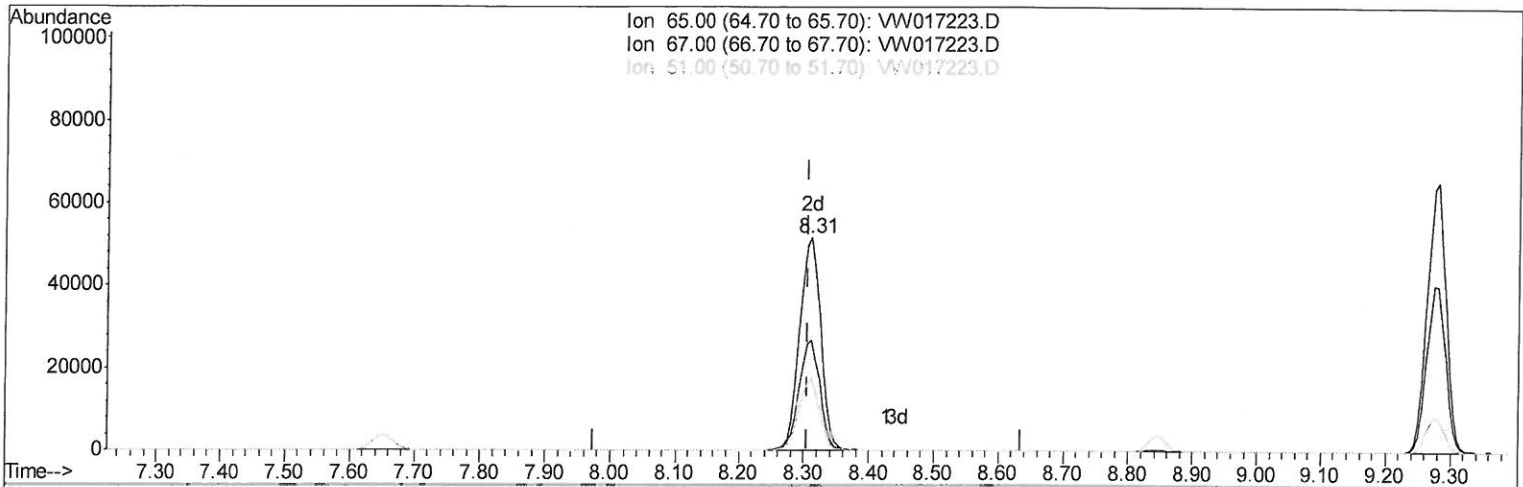

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+0.006) 21.97ug/L m

response 115507

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	0.05#
51.00	92.10	0.06#
0.00	0.00	0.00

11/18/2020

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
 Data File : VW017223.D
 Acq On : 13 Nov 2020 19:20
 Operator : SY/VA
 Sample : L4710-08
 Misc : 4.93G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AX7

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:51:27 PM

Quant Time: Nov 17 05:49:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	452906	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	377267	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	127890	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	119203	20.90	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.60%		
7) Chloroethane-d5	2.89	69	101969	23.20	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.80%		
10) 1,1-Dichloroethene-d2	4.02	63	166830	16.35	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.40%		
20) 2-Butanone-d5	7.08	46	26948	21.12	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	42.24%		
24) Chloroform-d	7.65	84	245232	23.19	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.76%		
26) 1,2-Dichloroethane-d4	8.31	65	115507m	21.97	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.88%		
29) Benzene-d6	8.28	84	482483	25.11	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.44%		
33) 1,2-Dichloropropane-d6	9.28	67	130988	24.65	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.60%		
37) Toluene-d8	10.33	98	447057	24.68	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.72%		
38) trans-1,3-Dichloropropene-	10.58	79	36226	15.12	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	60.48%		
39) 2-Hexanone-d5	10.93	63	20909	22.55	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	45.10%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	80787	17.45	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	69.80%		
61) 1,2-Dichlorobenzene-d4	13.86	152	99884	22.17	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	88.68%		
Target Compounds						
13) Acetone	4.13	43	3190	3.735	ug/L	78
16) Methylene chloride	4.93	84	20395	3.340	ug/L	97
43) 4-Methyl-2-pentanone	10.22	43	2267	0.793	ug/L #	93
44) Toluene	10.39	91	6312	0.289	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111320\
Data File : VW017223.D
Acq On : 13 Nov 2020 19:20
Operator : SY/VA
Sample : L4710-08
Misc : 4.93G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AX7

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:51:27 PM

Quant Time: Nov 17 05:49:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

