

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
 Data File : VW031007.D
 Acq On : 13 Nov 2024 13:20
 Operator : SY/MD
 Sample : P4751-13
 Misc : 5.56g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 14 00:31:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 14 00:30:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	381552	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	358977	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	158791	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	104269	16.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.640%
7) Chloroethane-d5	2.899	69	86231	17.967	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.880%
11) 1,1-Dichloroethene-d2	4.021	65	51764	20.047	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.200%
21) 2-Butanone-d5	7.075	46	45261	43.951	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.900%
24) Chloroform-d	7.648	84	248387	22.082	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.320%
26) 1,2-Dichloroethane-d4	8.301	65	121007	21.637	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.560%
32) Benzene-d6	8.276	84	486472	21.814	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.240%
36) 1,2-Dichloropropane-d6	9.270	67	145216	22.088	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.360%
41) Toluene-d8	10.325	98	430983	21.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.200%
43) trans-1,3-Dichloroprop...	10.575	79	51878	19.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.880%
47) 2-Hexanone-d5	10.922	63	37366	43.855	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	103689	22.638	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.560%
66) 1,2-Dichlorobenzene-d4	13.855	152	146048	25.250	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.000%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	3614	0.418	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
Data File : VW031007.D
Acq On : 13 Nov 2024 13:20
Operator : SY/MD
Sample : P4751-13
Misc : 5.56g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 14 00:31:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 14 00:30:57 2024
Response via : Initial Calibration

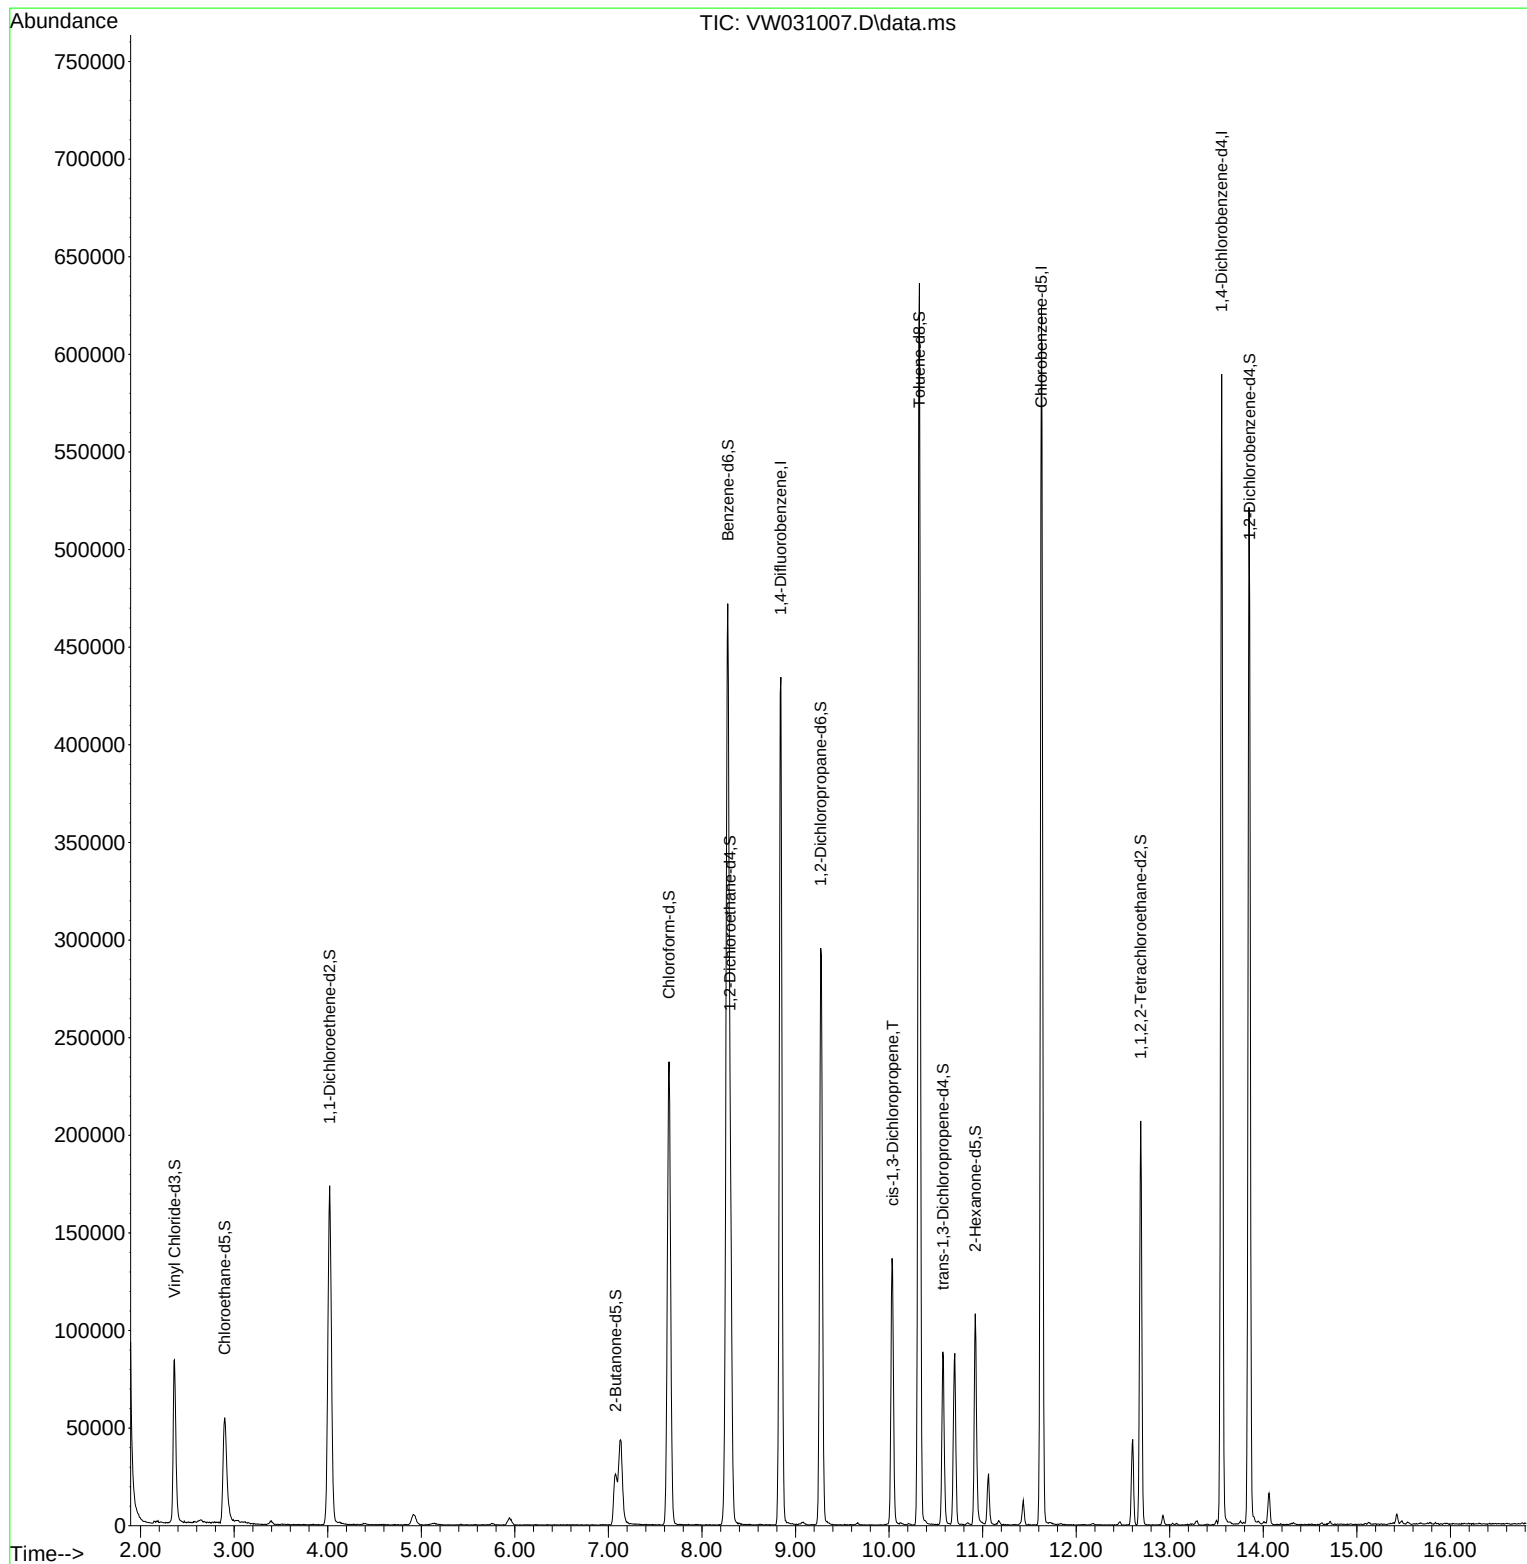

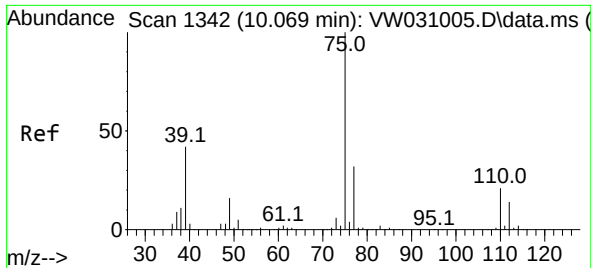

#39
 cis-1,3-Dichloropropene
 Concen: 0.418 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW031007.D
 Acq: 13 Nov 2024 13:20

Instrument :
 MSVOA_W
 ClientSampleId :

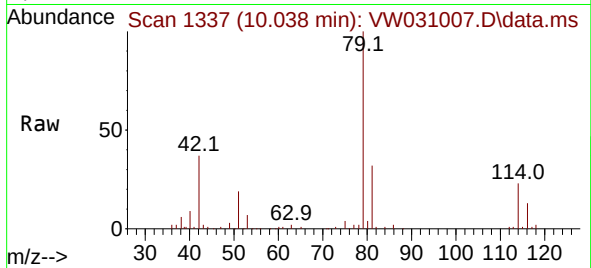

Tgt Ion: 75 Resp: 3614
 Ion Ratio Lower Upper
 75 100
 77 49.8 21.3 39.6#

