

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
 Data File : VW031008.D
 Acq On : 13 Nov 2024 13:44
 Operator : SY/MD
 Sample : P4751-17
 Misc : 5.80g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 14 00:32:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 14 00:30:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	392984	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	379421	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	163427	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	96565	14.982	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.920%
7) Chloroethane-d5	2.899	69	81537	16.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.960%
11) 1,1-Dichloroethene-d2	4.021	65	47249	17.766	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.080%
21) 2-Butanone-d5	7.075	46	52612	49.603	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.200%
24) Chloroform-d	7.648	84	247321	21.348	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.400%
26) 1,2-Dichloroethane-d4	8.307	65	124057	21.537	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.160%
32) Benzene-d6	8.276	84	477266	20.248	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.000%
36) 1,2-Dichloropropane-d6	9.276	67	144944	20.859	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.440%
41) Toluene-d8	10.325	98	418200	19.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.120%
43) trans-1,3-Dichloroprop...	10.581	79	53112	18.857	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.440%
47) 2-Hexanone-d5	10.922	63	43113	47.874	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	114094	23.567	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	151494	25.448	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.800%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	3486	0.381	ug/L	Qvalue # 48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
Data File : VW031008.D
Acq On : 13 Nov 2024 13:44
Operator : SY/MD
Sample : P4751-17
Misc : 5.80g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 14 00:32:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 14 00:30:57 2024
Response via : Initial Calibration

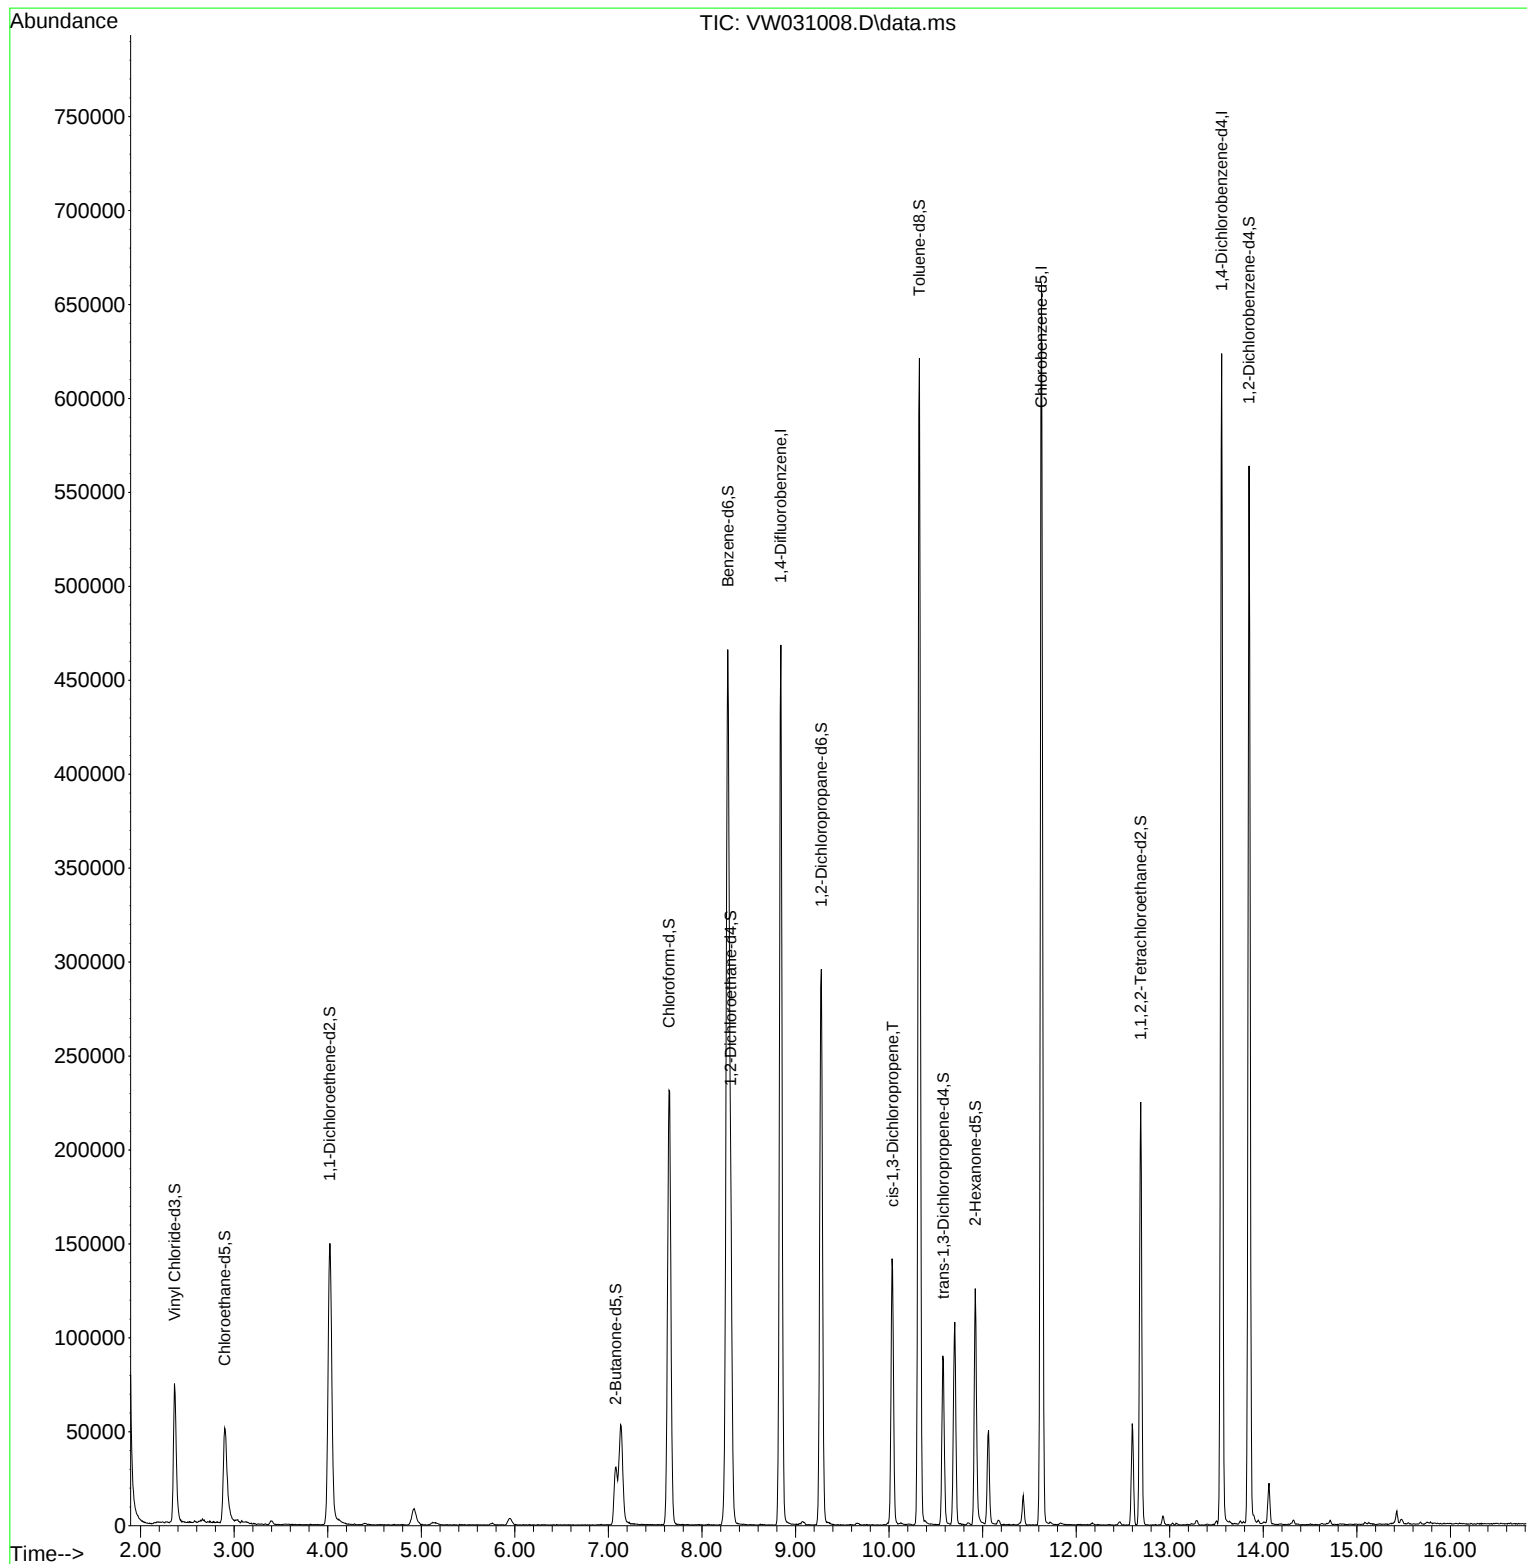

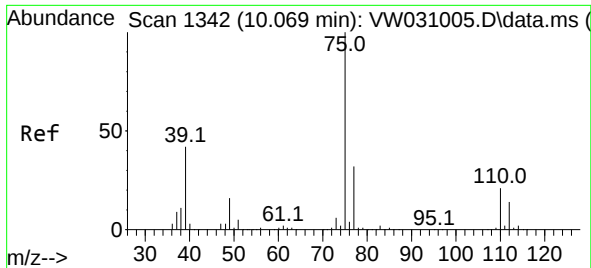

#39
 cis-1,3-Dichloropropene
 Concen: 0.381 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW031008.D
 Acq: 13 Nov 2024 13:44

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3486
 Ion Ratio Lower Upper
 75 100
 77 58.8 21.3 39.6#

