

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
 Data File : VW031010.D
 Acq On : 13 Nov 2024 14:31
 Operator : SY/MD
 Sample : P4751-21
 Misc : 4.77g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 14 00:32:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 14 00:30:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	395921	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	372673	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	169895	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	94267	14.517	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.080%		
7) Chloroethane-d5	2.899	69	80472	16.158	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.640%		
11) 1,1-Dichloroethene-d2	4.021	65	46776	17.458	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.840%		
21) 2-Butanone-d5	7.075	46	53849	50.392	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.780%		
24) Chloroform-d	7.648	84	246165	21.090	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.360%		
26) 1,2-Dichloroethane-d4	8.307	65	125109	21.558	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.240%		
32) Benzene-d6	8.270	84	466475	20.148	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	80.600%		
36) 1,2-Dichloropropane-d6	9.270	67	146769	21.504	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.000%		
41) Toluene-d8	10.319	98	419599	20.205	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.840%		
43) trans-1,3-Dichloroprop...	10.581	79	53623	19.383	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.520%		
47) 2-Hexanone-d5	10.922	63	45306	51.220	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.440%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	119620	25.156	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.640%		
66) 1,2-Dichlorobenzene-d4	13.848	152	150801	24.367	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.480%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3608	0.402	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111324\
Data File : VW031010.D
Acq On : 13 Nov 2024 14:31
Operator : SY/MD
Sample : P4751-21
Misc : 4.77g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 14 00:32:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 14 00:30:57 2024
Response via : Initial Calibration

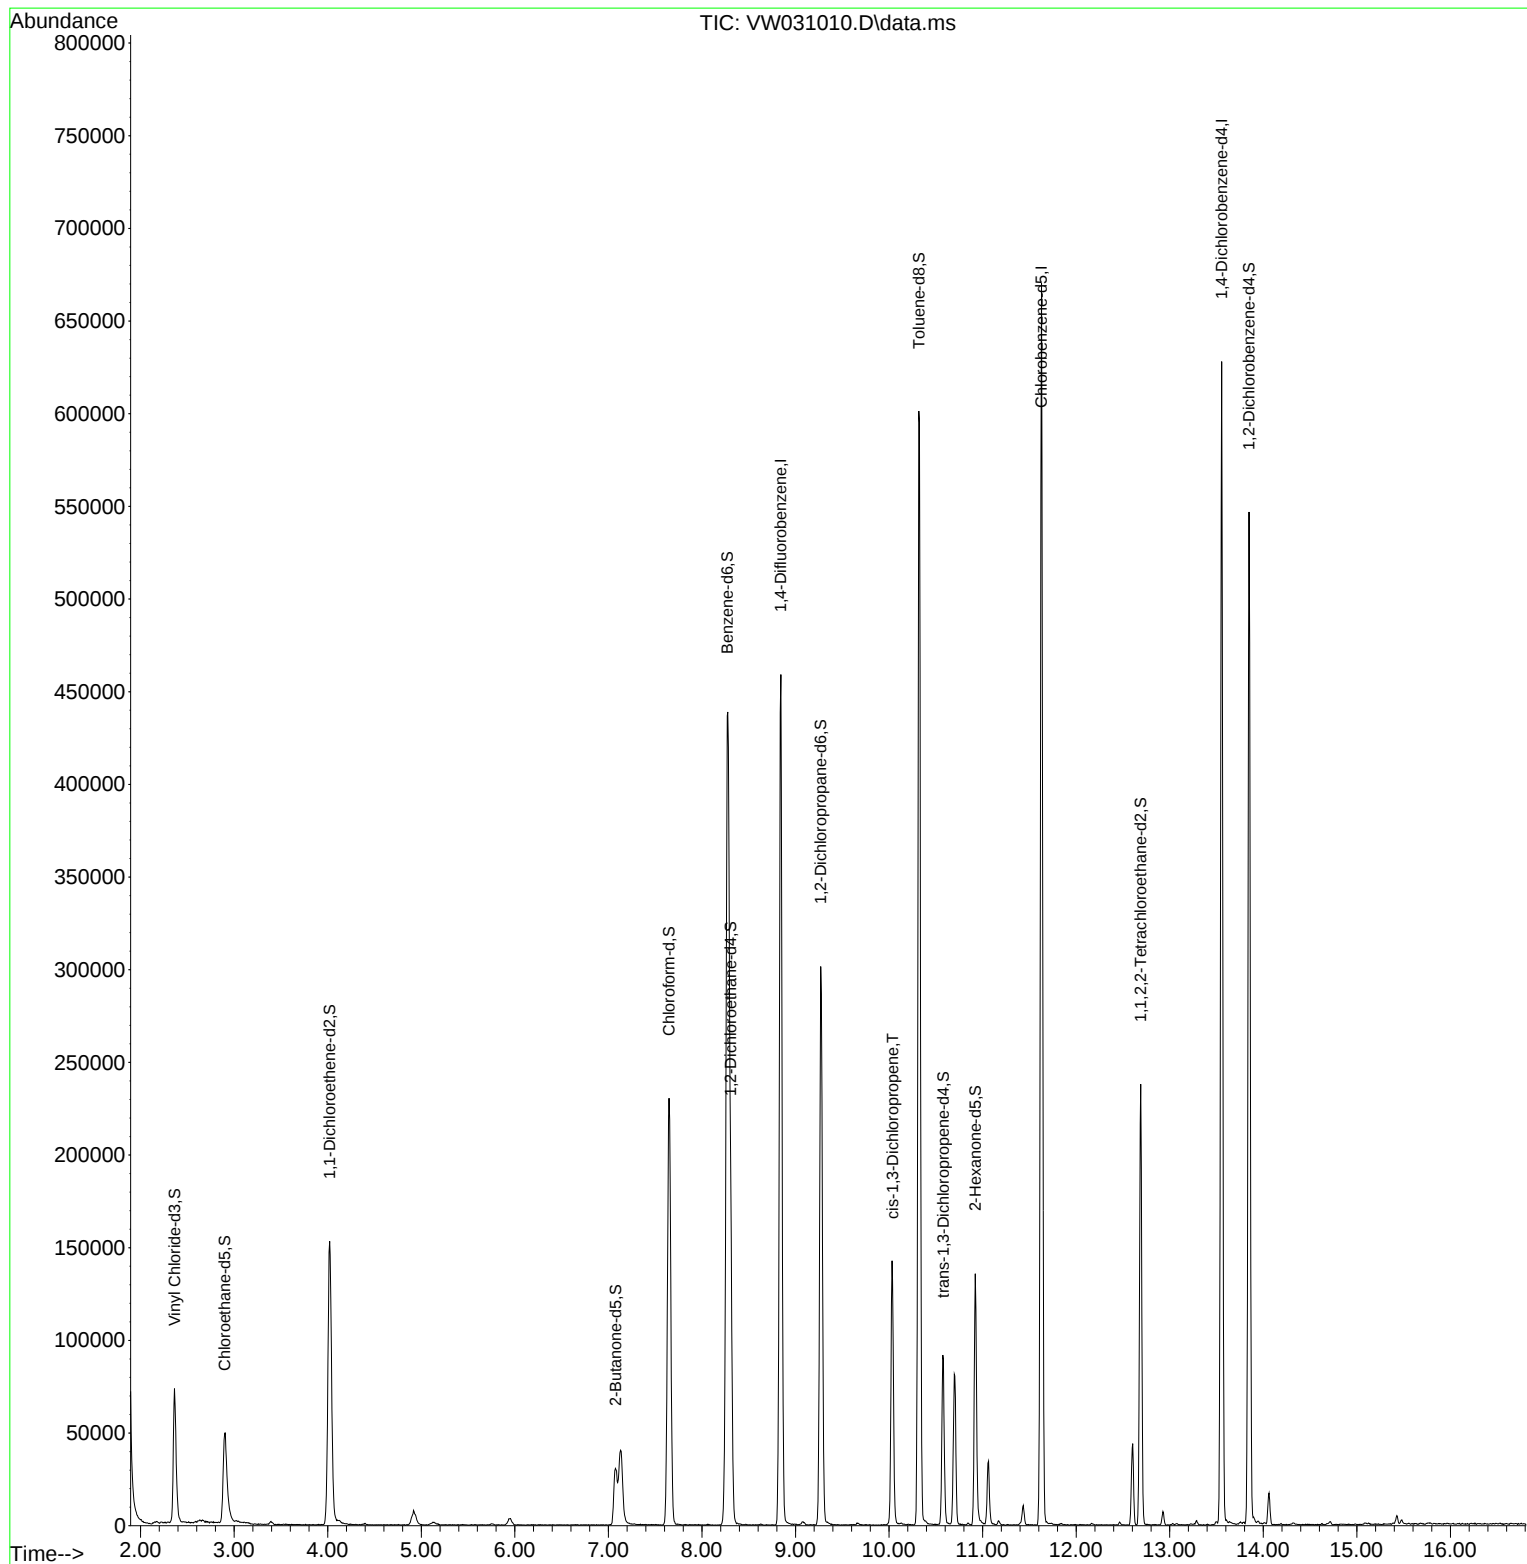

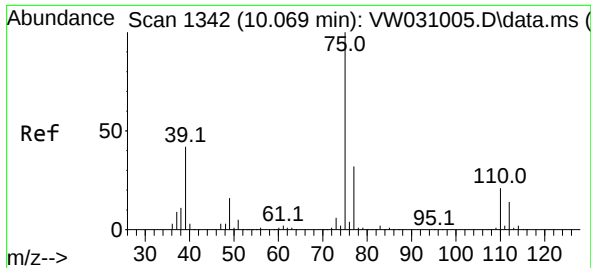

#39
 cis-1,3-Dichloropropene
 Concen: 0.402 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW031010.D
 Acq: 13 Nov 2024 14:31

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3608
 Ion Ratio Lower Upper
 75 100
 77 50.4 21.3 39.6#

