

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111419\
 Data File : VW014012.D
 Acq On : 14 Nov 2019 10:35
 Operator : SY/VA
 Sample : VW1114SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK23

Manual Integrations
 APPROVED

MMDadoda
 11/15/2019 9:44:26 AM

Quant Time: Nov 15 02:38:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 01:46:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	341944	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	335166	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	191001	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	137033	25.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.48%
7) Chloroethane-d5	2.89	69	106913	24.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.68%
10) 1,1-Dichloroethene-d2	4.02	63	204848	18.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.20%
20) 2-Butanone-d5	7.07	46	95762	60.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.84%
24) Chloroform-d	7.65	84	265151	25.22	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.88%
26) 1,2-Dichloroethane-d4	8.30	65	144309	27.30	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.20%
29) Benzene-d6	8.27	84	577077	24.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.08%
33) 1,2-Dichloropropane-d6	9.27	67	172430	24.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.00%
37) Toluene-d8	10.32	98	539038	23.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.60%
38) trans-1,3-Dichloropropene-	10.57	79	76407	25.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.44%
39) 2-Hexanone-d5	10.92	63	79997	60.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	151427	28.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	193095	25.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.64%

Target Compounds				Ovalue
13) Acetone	4.12	43	4333m	2.687 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111419\
Data File : VW014012.D
Acq On : 14 Nov 2019 10:35
Operator : SY/VA
Sample : VW1114SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleID :
VBLK23

Manual Integrations
APPROVED

MMDadoda
11/15/2019 9:44:26 AM

Quant Time: Nov 15 02:38:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 01:46:12 2019
Response via : Initial Calibration

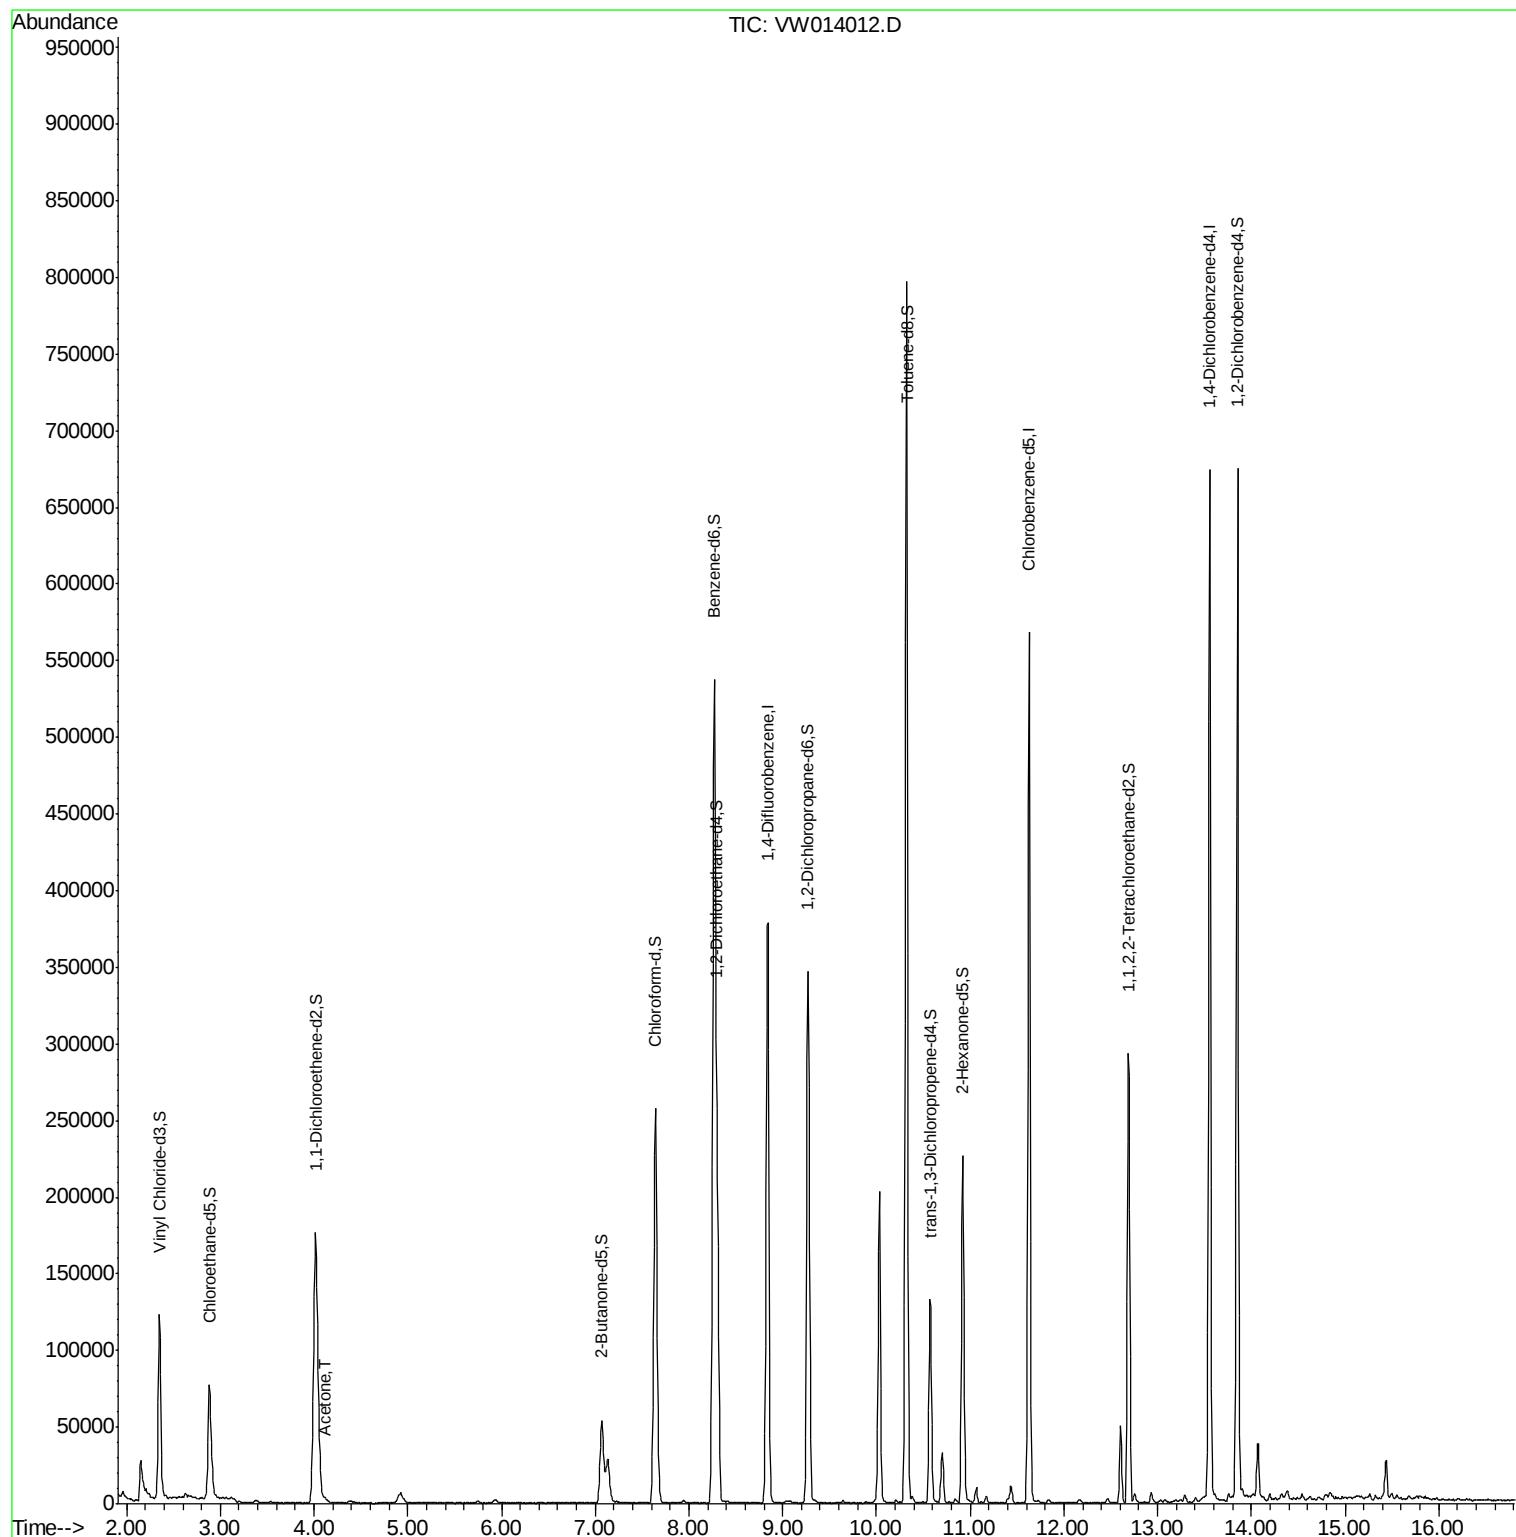

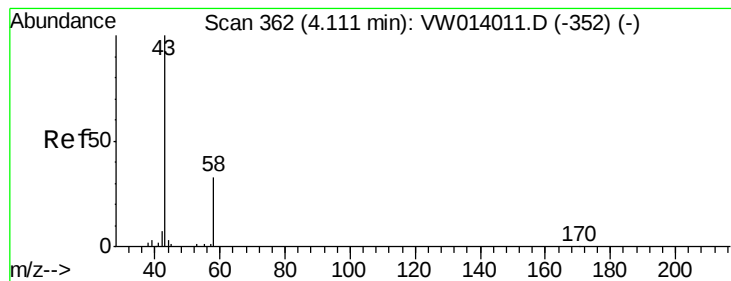

#13

Acetone

Concen: 2.687 ug/L m

RT: 4.12 min Scan# 363

Delta R.T. 0.01 min

Lab File: VW014012.D

Acq: 14 Nov 2019 10:35

Tot Ion: 43 Resp: 4333

Ion Ratio Lower Upper

43 100

58 18.7 0.0 65.4

Instrument :

MSVOA_W

ClientSampleId :

VBLK23

Manual Integrations

APPROVED

MMDadoda

11/15/2019 9:44:26 AM

