

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111419\
 Data File : VW014027.D
 Acq On : 14 Nov 2019 18:05
 Operator : SY/VA
 Sample : K5810-02
 Misc : 5.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFLY1

Quant Time: Nov 15 03:39:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 01:46:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	370892	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	358838	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	180042	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	122938	20.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.12%
7) Chloroethane-d5	2.88	69	105249	21.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.76%
10) 1,1-Dichloroethene-d2	4.02	63	195239	16.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.32%
20) 2-Butanone-d5	7.07	46	90273	52.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.02%
24) Chloroform-d	7.65	84	276543	24.25	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	8.30	65	153990	26.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.44%
29) Benzene-d6	8.27	84	600295	23.58	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.32%
33) 1,2-Dichloropropane-d6	9.27	67	181508	24.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.36%
37) Toluene-d8	10.32	98	547817	22.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.76%
38) trans-1,3-Dichloropropene-	10.57	79	73249	22.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.72%
39) 2-Hexanone-d5	10.92	63	70793	50.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	143126	25.41	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.64%
61) 1,2-Dichlorobenzene-d4	13.85	152	186798	25.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.28%


Target Compounds					Ovalue
35) Trichloroethene	9.09	95	31860	4.538 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111419\
Data File : VW014027.D
Acq On : 14 Nov 2019 18:05
Operator : SY/VA
Sample : K5810-02
Misc : 5.10G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFLY1

Quant Time: Nov 15 03:39:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 01:46:12 2019
Response via : Initial Calibration

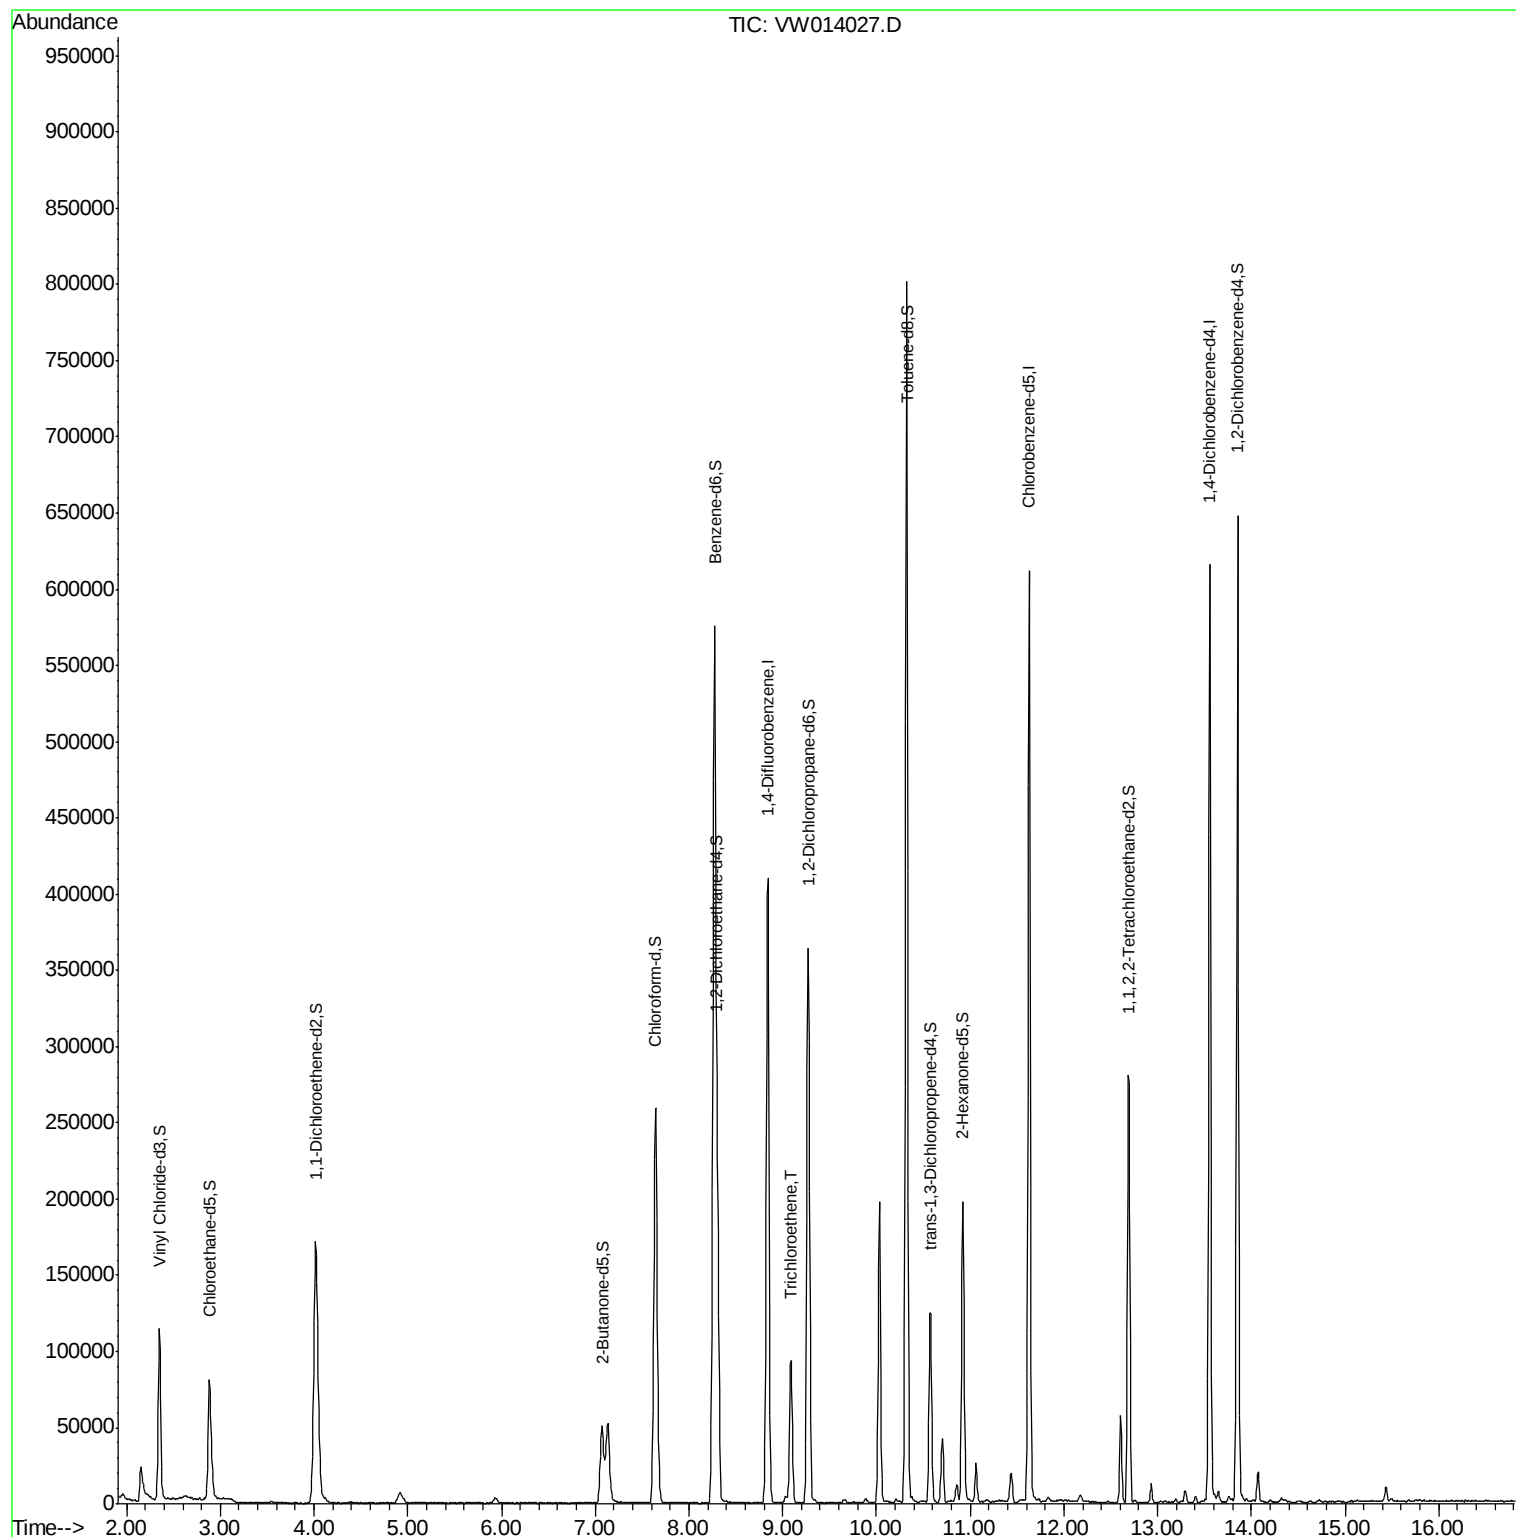


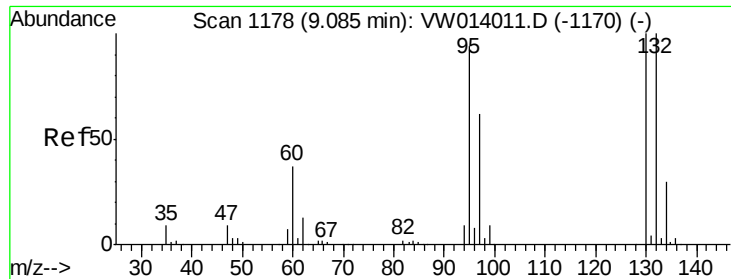

#35
 Trichloroethene
 Concen: 4.538 ug/L
 RT: 9.09 min Scan# 1178
 Delta R.T. -0.00 min
 Lab File: VW014027.D
 Acq: 14 Nov 2019 18:05

Instrument :
 MSVOA_W
 ClientSampleId :
 BFLY1

Tot Ion:	95	Resp:	31860
Ion	Ratio	Lower	Upper
95	100		
97	64.1	45.1	83.9
132	105.4	73.7	136.9
130	105.2	76.6	142.2

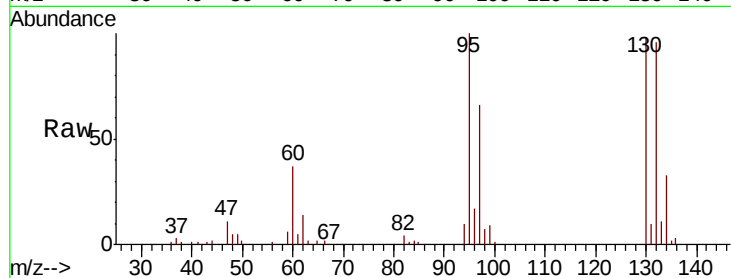

Abundance Ion 95.00 (94.70 to 95.70): VW
 Ion 97.00 (96.70 to 97.70): VW
 Ion 132.00 (131.70 to 132.70): V
 Ion 130.00 (129.70 to 130.70): V

