


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111618\
 Data File : VW006910.D
 Acq On : 16 Nov 2018 10:04
 Operator : SY/AP
 Sample : BFB83
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111418S.M
 Title : VOC Analysis
 Last Update : Fri Nov 16 23:51:03 2018

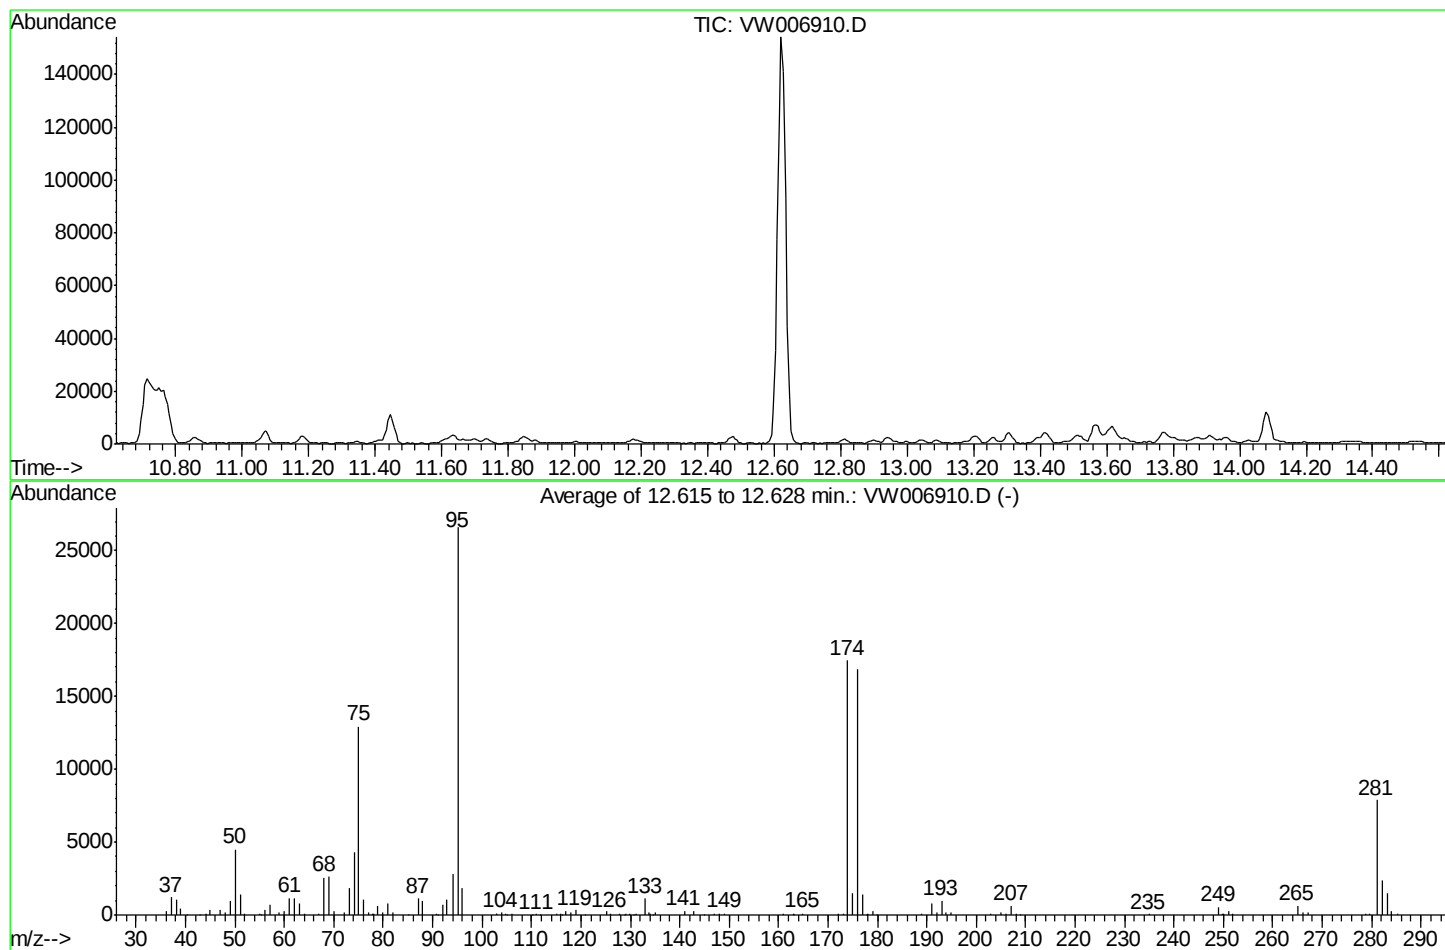

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4509	PASS
75	95	30	80	48.6	12911	PASS
95	95	100	100	100.0	26592	PASS
96	95	5	9	6.9	1835	PASS
173	174	0.00	2	0.6	106	PASS
174	95	50	120	65.6	17443	PASS
175	174	5	9	8.4	1459	PASS
176	174	95	101	96.8	16879	PASS
177	176	5	9	8.2	1378	PASS

Scan 1750 (12.573 min): VW006910.D
BFB83

m/z	Abundance
40.00	87.0
44.10	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.00	235.0
37.10	1143.0
38.10	975.0
39.00	376.0
40.00	109.0
42.90	73.0
44.00	234.0
45.00	357.0
47.10	287.0
48.00	142.0
49.00	863.0
50.00	3971.0
51.00	1244.0
52.10	86.0
55.00	72.0
56.00	372.0
57.10	697.0
59.00	247.0
59.90	181.0
61.00	1072.0
62.00	1031.0
63.00	691.0
64.10	61.0
67.00	65.0
68.00	2260.0
69.00	2228.0
70.10	286.0
72.10	194.0
73.10	2128.0
74.00	3841.0
75.10	11365.0
76.00	906.0
76.90	106.0
78.10	108.0
78.90	466.0
79.90	137.0
80.90	674.0
82.00	135.0
85.10	51.0
87.00	1024.0
88.00	759.0
90.80	64.0
92.00	638.0
93.00	955.0
94.10	2288.0
95.00	23064.0
96.00	1721.0
102.90	322.0
103.90	137.0
105.10	81.0
106.00	87.0
110.10	52.0
111.00	64.0
111.80	65.0
115.20	75.0
115.90	101.0
116.90	171.0
118.00	239.0
119.00	375.0
120.90	69.0
125.10	357.0
125.90	127.0
127.80	89.0
129.20	64.0
129.90	79.0
131.00	69.0
133.00	1530.0
133.90	247.0
134.50	138.0
135.00	113.0
140.90	267.0
142.90	152.0
144.90	57.0
146.90	157.0
148.00	78.0
149.10	178.0
160.90	110.0
162.90	115.0
164.90	131.0
173.10	319.0
174.00	13259.0
175.00	1272.0
176.00	12575.0
177.00	1052.0
177.80	84.0
179.00	303.0
179.80	51.0
189.00	89.0
191.00	844.0
192.00	156.0
193.00	1203.0
194.00	220.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

195.00	165.0
203.00	114.0
205.10	256.0
206.10	80.0
207.10	725.0
208.10	201.0
208.80	72.0
234.90	98.0
249.10	553.0
250.10	168.0
251.00	301.0
251.90	64.0
265.10	716.0
266.00	160.0
267.10	212.0
279.00	114.0
279.70	116.0
281.10	8343.0
282.10	2494.0
283.10	1739.0
284.10	386.0
285.20	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.00	328.0
37.00	1258.0
38.00	1207.0
39.00	402.0
40.20	83.0
43.00	53.0
44.10	141.0
45.00	464.0
47.00	339.0
48.00	221.0
49.10	1075.0
50.00	5067.0
51.00	1616.0
52.00	89.0
54.90	85.0
55.90	466.0
57.00	769.0
59.00	135.0
60.00	346.0
61.00	1407.0
62.10	1176.0
63.00	876.0
64.10	73.0
67.00	73.0
68.10	2783.0
69.00	3005.0
70.10	202.0
72.10	160.0
73.10	2009.0
74.10	4787.0
75.10	14403.0
76.10	1210.0
77.00	167.0
78.20	74.0
79.00	697.0
79.90	270.0
80.90	903.0
82.00	125.0
87.00	1124.0
88.00	1046.0
91.10	75.0
92.00	590.0
93.00	1262.0
94.00	3348.0
95.10	29360.0
96.10	1950.0
103.10	169.0
104.00	194.0
104.80	131.0
105.90	152.0
110.10	81.0
111.00	51.0
115.10	86.0
116.10	114.0
117.00	349.0
118.00	153.0
118.90	356.0
125.10	292.0
125.80	78.0
127.90	99.0
129.10	84.0
129.80	127.0
130.70	77.0
133.10	1149.0
134.10	181.0
135.10	146.0
140.80	363.0
142.90	315.0
147.00	131.0
148.00	61.0
149.00	147.0
160.90	72.0
163.10	206.0
164.90	155.0
172.10	83.0
174.00	19376.0
175.00	1616.0
176.00	18720.0
177.00	1398.0
178.00	153.0
179.10	191.0
189.10	66.0
191.10	979.0
192.00	262.0
193.10	997.0
194.00	207.0
195.00	171.0
203.00	121.0
205.00	216.0
206.00	67.0
207.20	694.0
208.10	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

235.00	67.0
249.00	603.0
249.80	122.0
250.10	131.0
251.10	315.0
252.00	86.0
265.10	759.0
265.90	193.0
267.00	254.0
278.90	94.0
279.50	125.0
281.10	8562.0
282.10	2690.0
283.10	1545.0
284.10	317.0
285.20	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.00	279.0
37.00	1180.0
38.10	999.0
39.10	507.0
40.00	121.0
44.00	237.0
45.00	309.0
47.00	422.0
48.00	183.0
49.00	998.0
50.10	4489.0
51.00	1357.0
51.90	62.0
54.80	52.0
55.20	71.0
55.90	311.0
57.10	703.0
59.10	106.0
60.00	212.0
61.00	1053.0
62.10	1176.0
63.00	921.0
64.10	75.0
66.90	55.0
68.10	2632.0
69.00	2631.0
70.10	218.0
72.00	195.0
73.10	1404.0
74.00	4401.0
75.00	12967.0
76.10	1036.0
77.00	168.0
77.80	149.0
79.00	738.0
79.90	170.0
81.00	673.0
82.00	209.0
87.00	1165.0
88.00	1046.0
90.90	144.0
92.00	799.0
92.90	1011.0
94.00	2893.0
95.10	27352.0
96.10	1834.0
103.00	188.0
103.90	152.0
104.90	92.0
105.90	119.0
111.00	54.0
115.20	80.0
115.70	96.0
117.00	199.0
118.10	267.0
119.00	261.0
125.10	216.0
126.00	87.0
127.90	96.0
128.90	56.0
129.80	87.0
130.60	54.0
131.10	96.0
133.00	711.0
133.80	225.0
135.00	163.0
141.00	289.0
142.90	303.0
147.00	55.0
148.00	91.0
149.00	51.0
161.00	82.0
163.00	108.0
165.00	72.0
172.10	88.0
174.00	19696.0
175.00	1489.0
176.00	19344.0
177.00	1686.0
179.00	233.0
191.00	630.0
192.10	164.0
193.00	768.0
193.90	216.0
195.10	82.0
202.80	56.0
205.10	185.0
207.10	561.0
208.20	63.0
235.00	80.0
249.00	541.0
249.90	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

251.00	243.0
252.00	96.0
265.10	486.0
266.10	159.0
267.20	111.0
279.50	92.0
281.10	6702.0
282.10	1887.0
283.10	1290.0
284.20	149.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83