




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
Data File : VW020904.D
Acq On : 16 Nov 2021 11:33
Operator : SY/VA
Sample : VIBLK493
Misc : 5.00g/10.00mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 17 00:25:49 2021
Response via : Initial Calibration

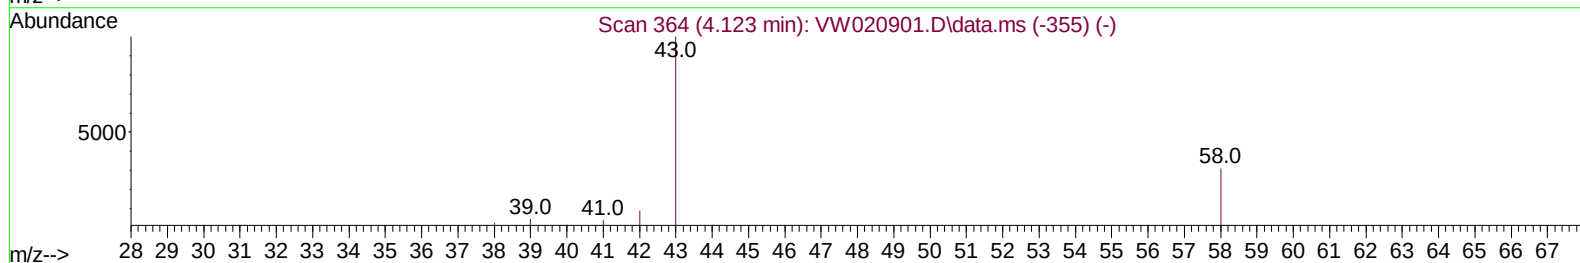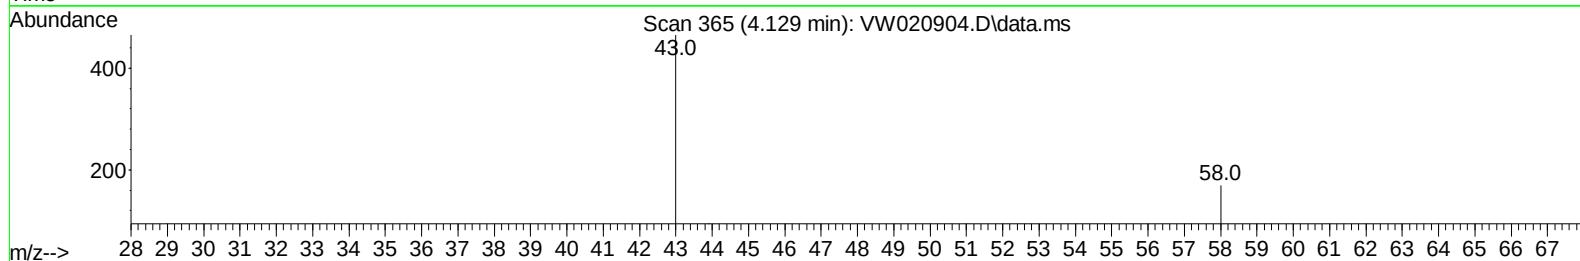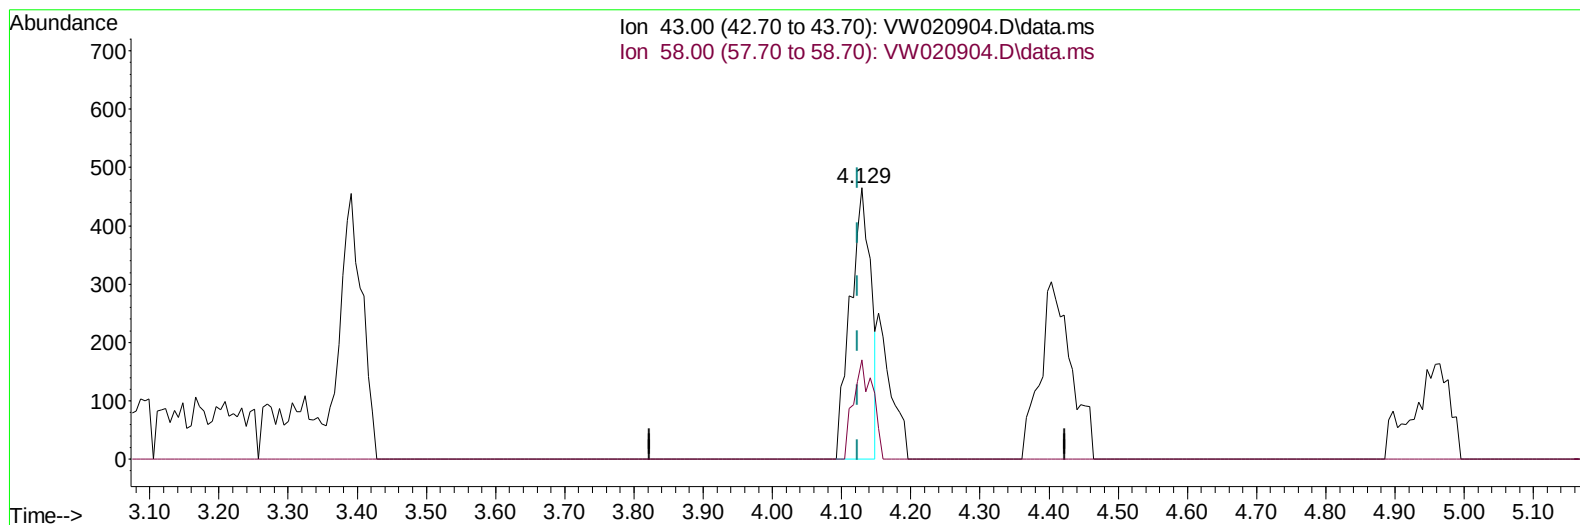

TIC: VW020904.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.02 ug/L

response 958

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	22.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
Data File : VW020904.D
Acq On : 16 Nov 2021 11:33
Operator : SY/VA
Sample : VIBLK493
Misc : 5.00g/10.00mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 17 00:25:49 2021
Response via : Initial Calibration

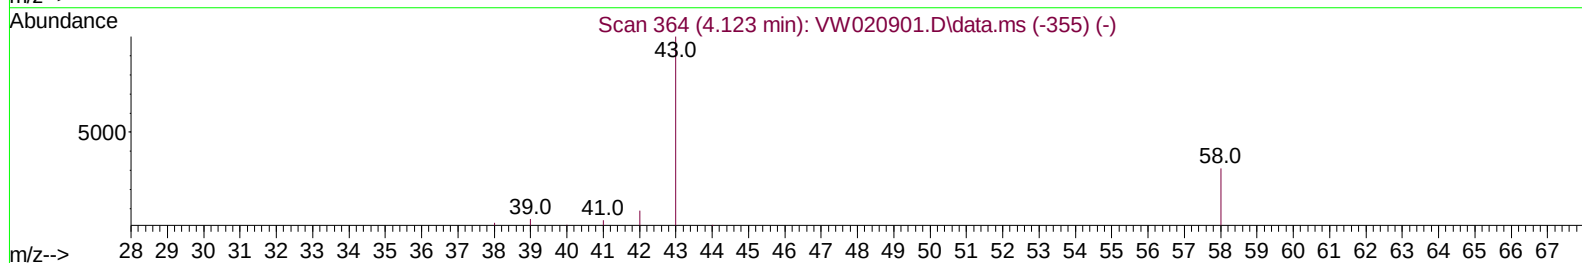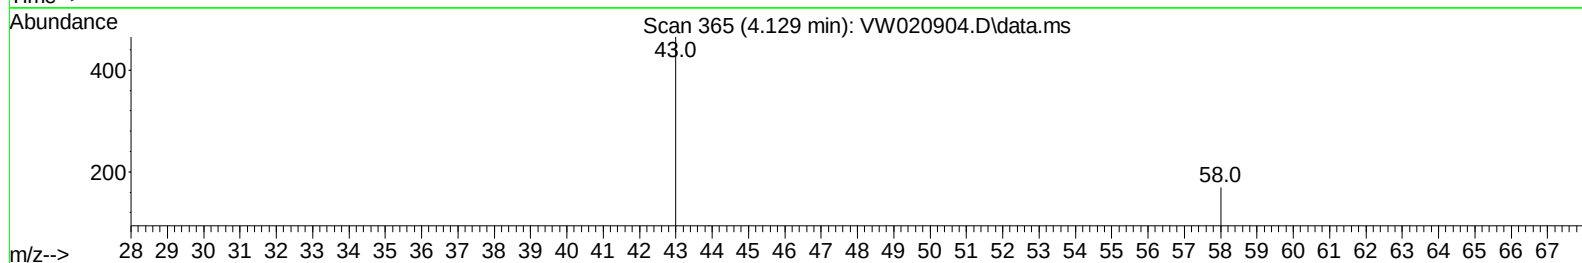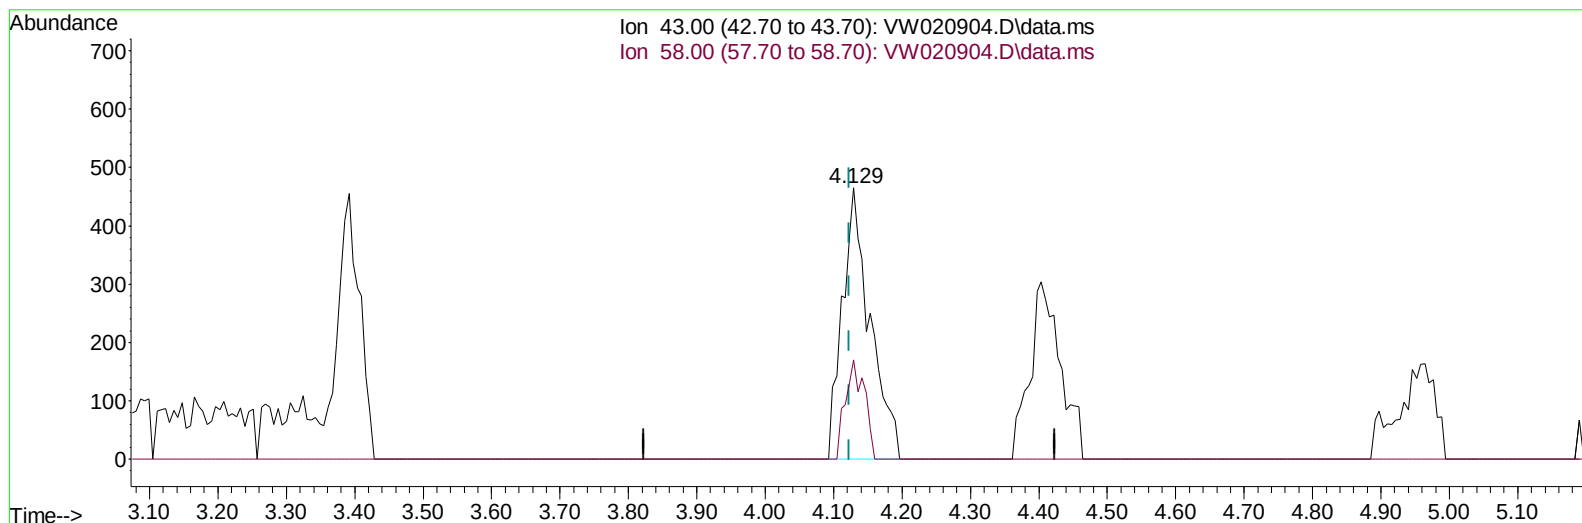

TIC: VW020904.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.13 ug/L m

response 1309

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	16.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw111621\
 Data File : VW020904.D
 Acq On : 16 Nov 2021 11:33
 Operator : SY/VA
 Sample : VIBLK493
 Misc : 5.00g/10.00mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 17 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		122720	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		110545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		61375	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		32032	22.503	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	90.000%	
7) Chloroethane-d5	2.892	69		21263	23.161	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	92.640%	
11) 1,1-Dichloroethene-d2	4.019	63		46479	16.876	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.520%	
21) 2-Butanone-d5	7.086	46		13756	38.716	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery	=	77.440%	
24) Chloroform-d	7.647	84		63881	20.659	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	82.640%	
26) 1,2-Dichloroethane-d4	8.305	65		33055	21.061	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	84.240%	
32) Benzene-d6	8.281	84		128600	22.072	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	88.280%	
36) 1,2-Dichloropropane-d6	9.275	67		35777	21.564	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	86.240%	
41) Toluene-d8	10.323	98		127029	21.967	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	87.880%	
43) trans-1,3-Dichloroprop...	10.579	79		16046	20.462	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	81.840%	
47) 2-Hexanone-d5	10.927	63		10948	39.787	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	79.580%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84		25416	19.998	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	80.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152		46548	21.279	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	85.120%	
Target Compounds							
13) Acetone	4.129	43		1309m	4.126	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
Data File : VW020904.D
Acq On : 16 Nov 2021 11:33
Operator : SY/VA
Sample : VIBLK493
Misc : 5.00g/10.00mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 17 00:25:49 2021
Response via : Initial Calibration

