

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
 Data File : VW020904.D
 Acq On : 16 Nov 2021 11:33
 Operator : SY/VA
 Sample : VIBLK493
 Misc : 5.00g/10.00mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 17 00:25:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	122720	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	110545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	61375	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	32032	22.503	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.000%		
7) Chloroethane-d5	2.892	69	21263	23.161	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.640%		
11) 1,1-Dichloroethene-d2	4.019	63	46479	16.876	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.520%		
21) 2-Butanone-d5	7.086	46	13756	38.716	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.440%		
24) Chloroform-d	7.647	84	63881	20.659	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.640%		
26) 1,2-Dichloroethane-d4	8.305	65	33055	21.061	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.240%		
32) Benzene-d6	8.281	84	128600	22.072	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.280%		
36) 1,2-Dichloropropane-d6	9.275	67	35777	21.564	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.240%		
41) Toluene-d8	10.323	98	127029	21.967	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.880%		
43) trans-1,3-Dichloroprop...	10.579	79	16046	20.462	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.840%		
47) 2-Hexanone-d5	10.927	63	10948	39.787	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.580%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	25416	19.998	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.000%		
66) 1,2-Dichlorobenzene-d4	13.853	152	46548	21.279	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.120%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	1309m	4.126	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
Data File : VW020904.D
Acq On : 16 Nov 2021 11:33
Operator : SY/VA
Sample : VIBLK493
Misc : 5.00g/10.00mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK493

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 00:27:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 17 00:25:49 2021
Response via : Initial Calibration

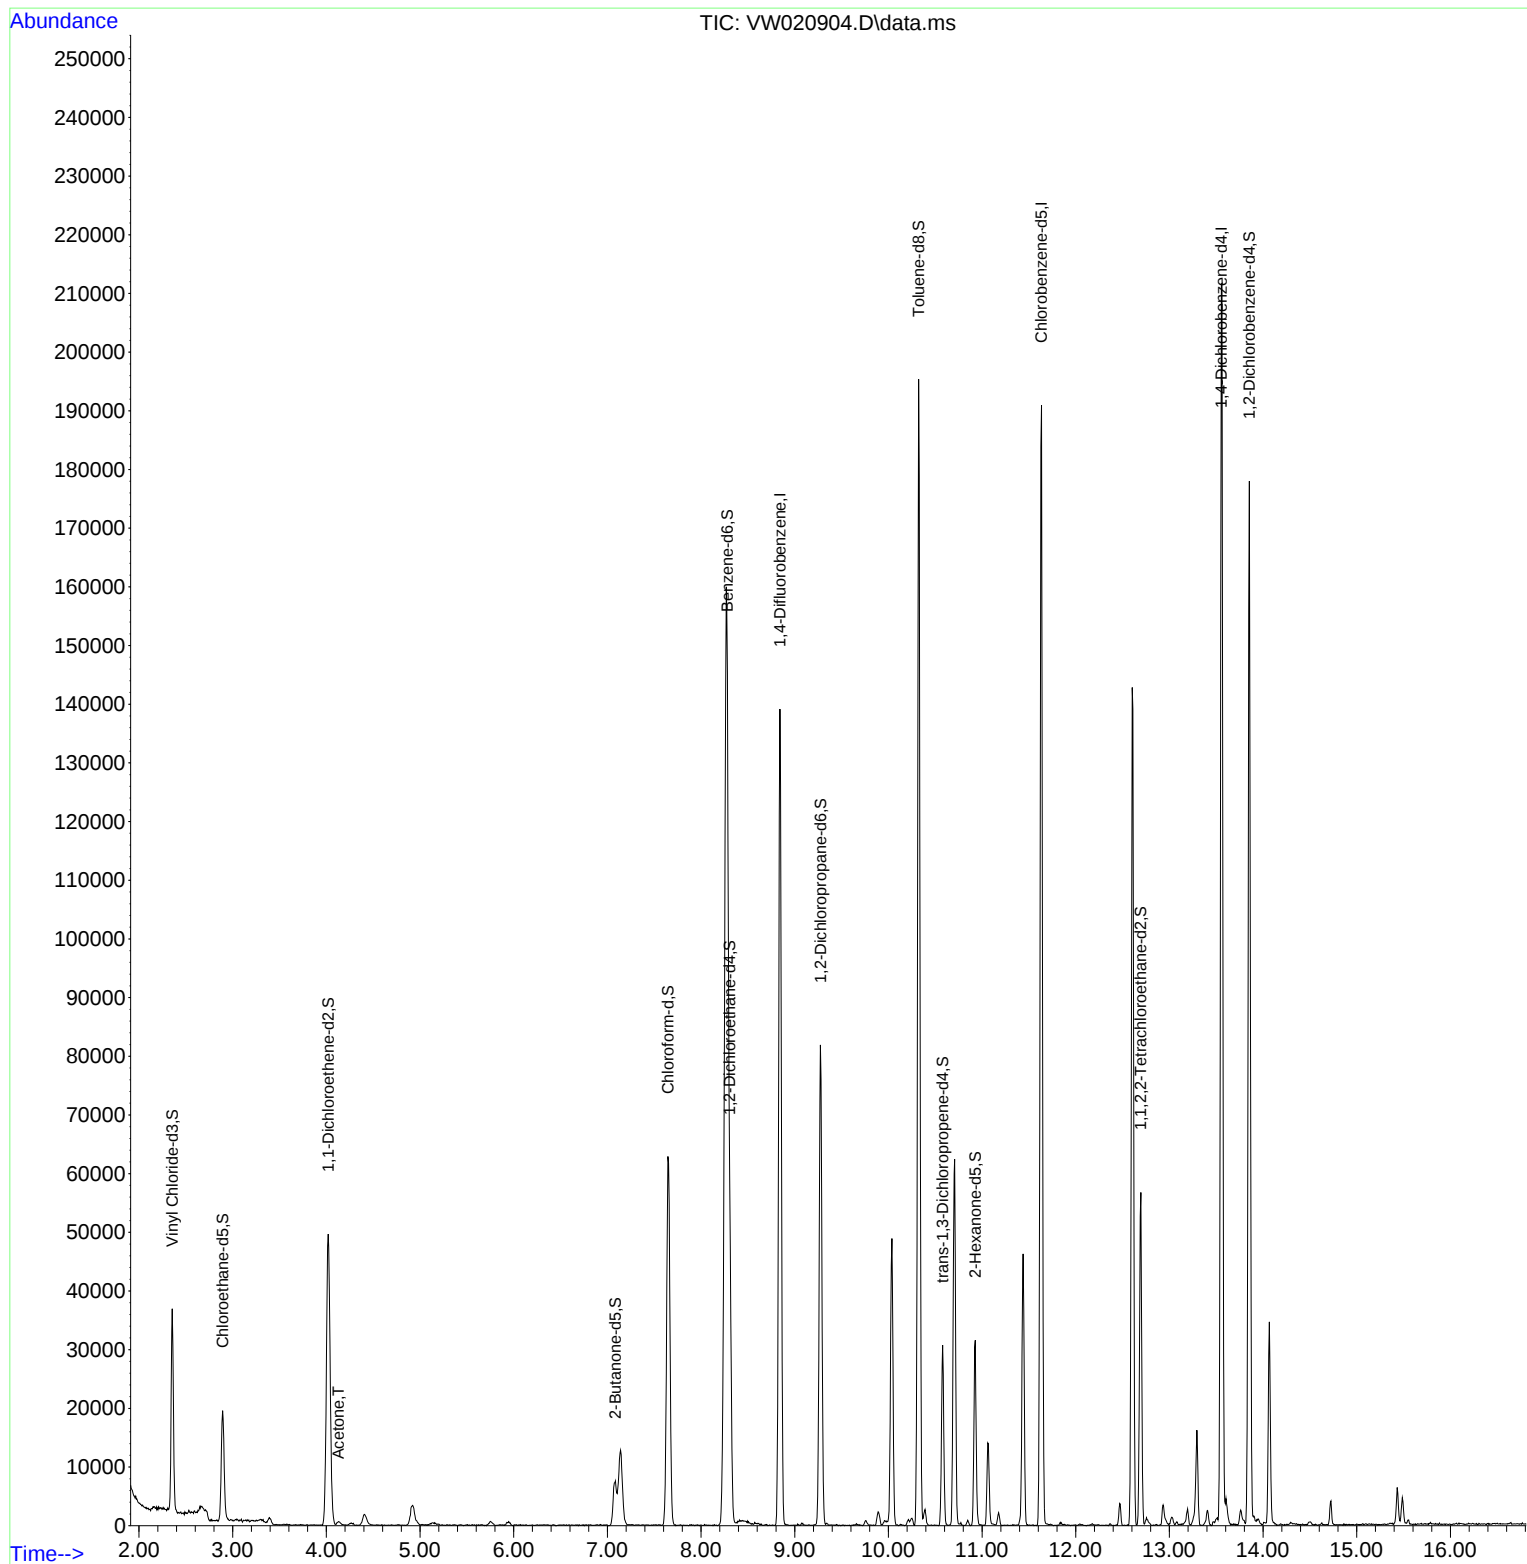

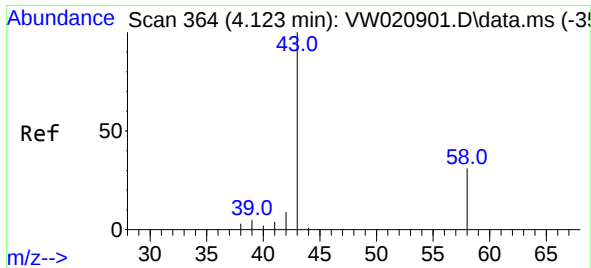

#13
 Acetone
 Concen: 4.126 ug/L m
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW020904.D
 Acq: 16 Nov 2021 11:33

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK493

Tgt Ion: 43 Resp: 1309
 Ion Ratio Lower Upper
 43 100
 58 16.7 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

