
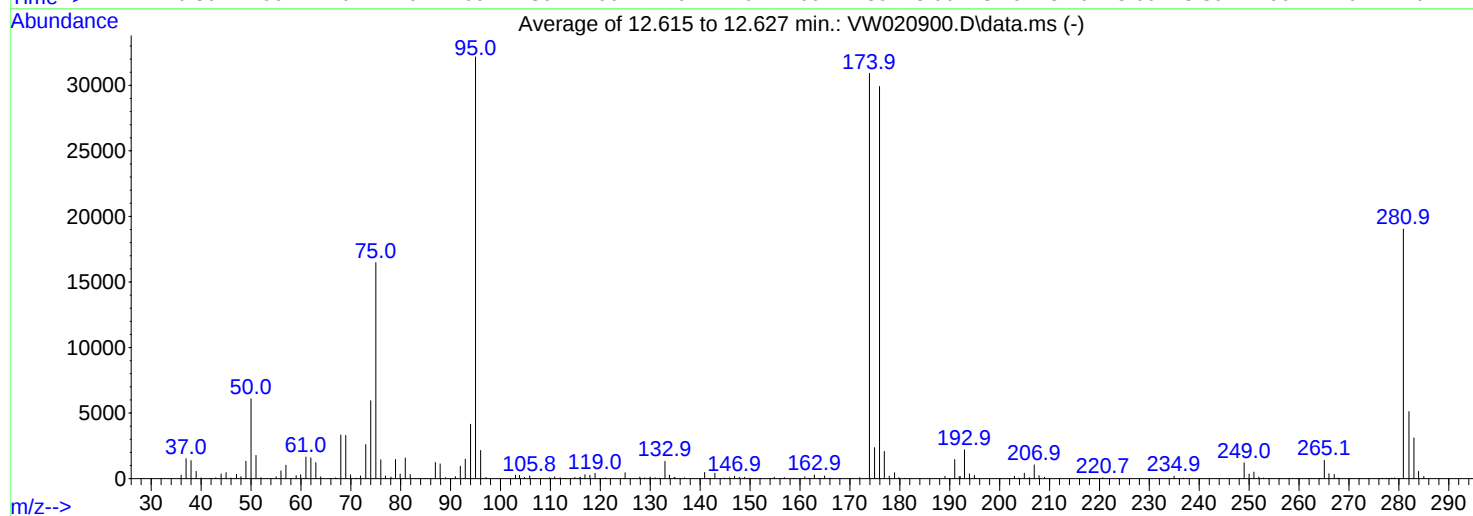


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111621\
 Data File : VW020900.D
 Acq On : 16 Nov 2021 07:43
 Operator : SY/VA
 Sample : BFB464
 Misc : 5.00g/10.00mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB464

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Title : SFAM01.0
 Last Update : Wed Nov 17 00:25:49 2021

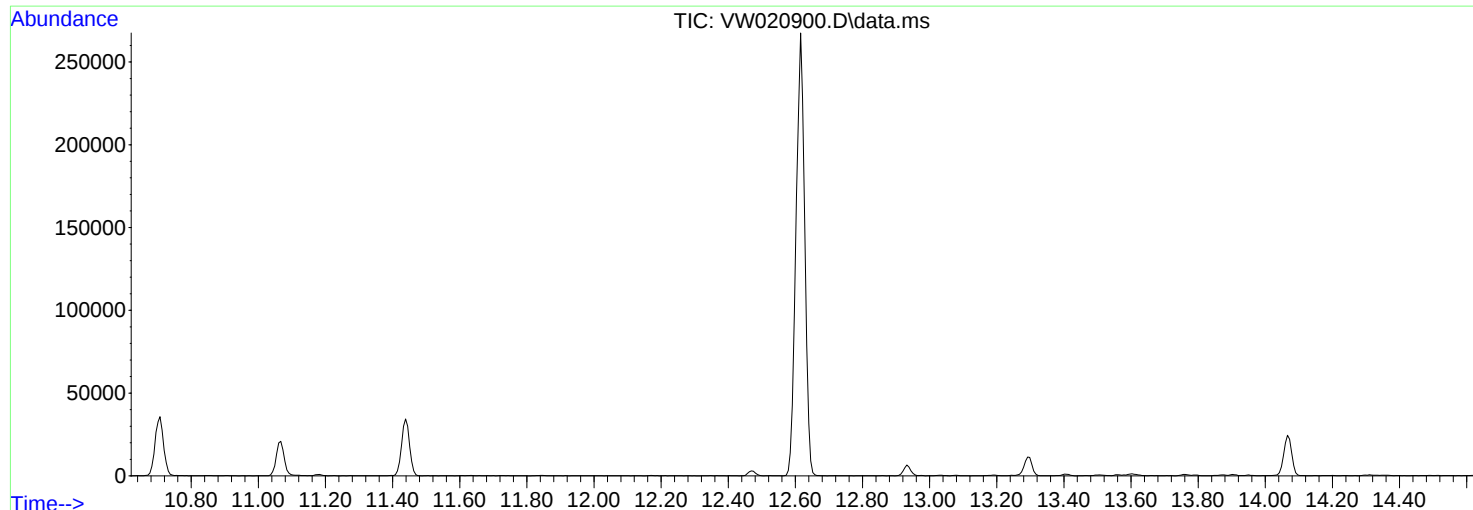

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6097	PASS
75	95	30	80	51.2	16481	PASS
95	95	100	100	100.0	32171	PASS
96	95	5	9	6.7	2155	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.1	30909	PASS
175	174	5	9	7.7	2371	PASS
176	174	95	105	96.8	29907	PASS
177	176	5	10	6.9	2070	PASS

m/z	Abundance
57.00	75.0
73.00	107.0
280.90	178.0
282.00	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

m/z	Abundance
36.00	306.0
37.00	1866.0
38.00	1649.0
39.00	609.0
40.00	52.0
43.00	130.0
44.00	355.0
45.00	711.0
46.10	77.0
47.10	387.0
48.10	165.0
49.00	1531.0
50.00	6952.0
51.00	1900.0
52.00	102.0
55.10	104.0
56.00	756.0
57.00	1379.0
58.00	55.0
59.10	460.0
59.90	316.0
61.00	2014.0
62.00	1826.0
63.00	1317.0
64.00	174.0
66.90	100.0
68.00	3473.0
69.00	3464.0
69.90	335.0
71.10	53.0
72.00	262.0
73.00	3947.0
74.00	6946.0
75.00	17752.0
76.00	1727.0
77.00	226.0
78.00	153.0
78.90	1528.0
79.90	377.0
80.90	1737.0
81.90	340.0
83.00	69.0
83.70	64.0
84.90	80.0
86.90	1347.0
87.90	1283.0
89.00	153.0
90.90	172.0
92.00	1022.0
93.00	1576.0
94.00	4417.0
95.00	33312.0
96.00	2376.0
97.00	136.0
103.00	544.0
103.90	366.0
104.80	192.0
105.90	256.0
106.90	58.0
109.90	165.0
110.90	209.0
111.90	152.0
113.00	73.0
114.90	151.0
115.80	171.0
117.00	324.0
117.90	330.0
119.00	635.0
119.80	73.0
121.00	122.0
125.00	698.0
127.90	133.0
129.90	147.0
131.00	134.0
131.90	108.0
132.90	2242.0
133.90	463.0
134.80	215.0
136.90	73.0
140.90	494.0
143.00	467.0
144.90	105.0
145.90	141.0
146.90	283.0
147.80	145.0
148.90	185.0
149.80	98.0
151.00	53.0
154.90	99.0
156.80	84.0
158.80	75.0
161.00	217.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

161.80	72.0
162.90	466.0
163.80	89.0
164.90	331.0
166.00	149.0
173.90	31552.0
175.00	2241.0
175.90	31040.0
176.90	2003.0
177.90	314.0
178.90	864.0
179.80	182.0
180.90	79.0
189.00	346.0
191.00	2500.0
191.90	493.0
192.90	3703.0
194.00	664.0
194.90	461.0
195.90	57.0
203.00	250.0
203.90	100.0
204.90	749.0
206.00	224.0
207.00	1791.0
207.90	395.0
209.00	196.0
219.00	66.0
220.80	117.0
235.00	373.0
236.00	81.0
236.90	70.0
249.00	2144.0
250.00	606.0
250.90	842.0
251.90	248.0
252.90	82.0
265.10	2476.0
266.00	685.0
267.00	529.0
267.80	153.0
276.70	63.0
277.60	71.0
281.00	37552.0
282.00	9582.0
283.00	5241.0
283.90	851.0
285.10	265.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

m/z	Abundance
36.00	299.0
37.00	1594.0
38.00	1515.0
39.00	643.0
40.00	68.0
42.90	101.0
44.00	445.0
45.00	436.0
45.90	65.0
47.10	346.0
48.00	159.0
49.00	1475.0
50.00	6912.0
51.00	2081.0
52.00	132.0
55.00	107.0
55.10	107.0
56.00	580.0
57.10	1134.0
58.90	162.0
60.00	329.0
61.00	1616.0
62.00	1697.0
63.00	1436.0
63.90	113.0
67.10	81.0
68.00	3876.0
69.00	3838.0
70.00	341.0
71.10	51.0
71.90	190.0
73.00	2553.0
74.00	6378.0
75.00	18472.0
76.00	1605.0
77.00	223.0
78.10	89.0
78.90	1574.0
79.90	381.0
80.90	1723.0
81.90	389.0
86.90	1409.0
87.90	1272.0
88.80	78.0
91.00	177.0
92.00	1062.0
93.00	1596.0
94.00	4691.0
95.00	35880.0
96.00	2454.0
97.10	94.0
103.00	176.0
103.70	239.0
104.80	101.0
105.90	225.0
109.80	61.0
110.80	120.0
112.00	79.0
114.90	154.0
116.00	218.0
116.90	373.0
117.90	310.0
118.90	334.0
121.00	53.0
124.90	519.0
127.90	137.0
128.90	84.0
129.90	126.0
130.90	74.0
132.10	55.0
133.00	1262.0
133.80	240.0
135.00	182.0
136.80	85.0
140.90	500.0
141.80	66.0
143.00	447.0
144.80	57.0
145.90	83.0
146.90	170.0
147.90	89.0
148.90	102.0
154.90	108.0
156.80	93.0
159.00	51.0
160.90	167.0
162.90	274.0
165.00	205.0
172.00	128.0
173.90	34544.0
174.90	2792.0
176.00	33624.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

176.90	2383.0
177.90	200.0
179.00	390.0
179.90	53.0
189.10	135.0
190.00	56.0
191.00	1418.0
192.10	325.0
193.00	2165.0
193.90	278.0
195.00	224.0
202.90	200.0
203.90	53.0
205.00	394.0
205.70	63.0
206.90	939.0
207.90	214.0
209.00	133.0
218.90	51.0
220.60	79.0
234.90	150.0
236.80	60.0
249.00	1048.0
250.00	270.0
251.00	434.0
252.00	125.0
252.90	53.0
264.20	71.0
265.00	1151.0
266.00	329.0
267.10	292.0
268.00	87.0
278.10	62.0
278.60	110.0
279.20	186.0
280.90	13297.0
282.00	3716.0
283.00	3122.0
284.00	563.0
284.90	181.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

m/z	Abundance
35.90	193.0
37.10	1105.0
38.10	962.0
39.00	419.0
40.00	66.0
44.00	266.0
45.00	255.0
47.10	250.0
47.90	139.0
49.00	997.0
50.00	4427.0
51.00	1325.0
55.10	118.0
56.00	449.0
57.00	791.0
58.90	65.0
59.90	234.0
61.00	1316.0
62.00	1253.0
63.00	900.0
64.00	104.0
66.90	77.0
68.00	2658.0
69.00	2587.0
69.90	222.0
72.00	182.0
73.00	1635.0
74.00	4515.0
75.00	13220.0
76.00	987.0
76.90	156.0
78.10	137.0
79.00	1294.0
79.90	299.0
80.90	1251.0
81.80	236.0
87.00	953.0
88.00	814.0
90.90	114.0
91.90	793.0
92.90	1310.0
94.00	3335.0
95.00	27320.0
96.00	1636.0
97.20	77.0
103.00	72.0
103.80	135.0
105.80	164.0
110.80	69.0
116.00	103.0
116.80	218.0
117.90	132.0
118.90	230.0
124.80	129.0
127.90	115.0
128.90	85.0
130.00	109.0
133.10	466.0
134.00	98.0
134.80	112.0
136.80	64.0
140.90	427.0
142.90	331.0
146.80	84.0
147.90	81.0
148.80	65.0
154.80	127.0
156.90	68.0
161.00	66.0
162.80	90.0
164.90	99.0
171.90	108.0
173.90	26632.0
174.90	2081.0
175.90	25056.0
176.90	1823.0
177.80	83.0
178.80	104.0
189.00	56.0
191.00	431.0
192.10	173.0
193.00	741.0
194.00	176.0
194.80	86.0
203.00	114.0
205.10	109.0
207.00	404.0
208.00	88.0
234.80	68.0
248.90	452.0
250.00	186.0
250.90	219.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464

265.00	595.0
266.00	136.0
266.90	125.0
278.80	65.0
281.00	6796.0
282.00	2216.0
283.00	982.0
283.90	249.0
285.00	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB464