



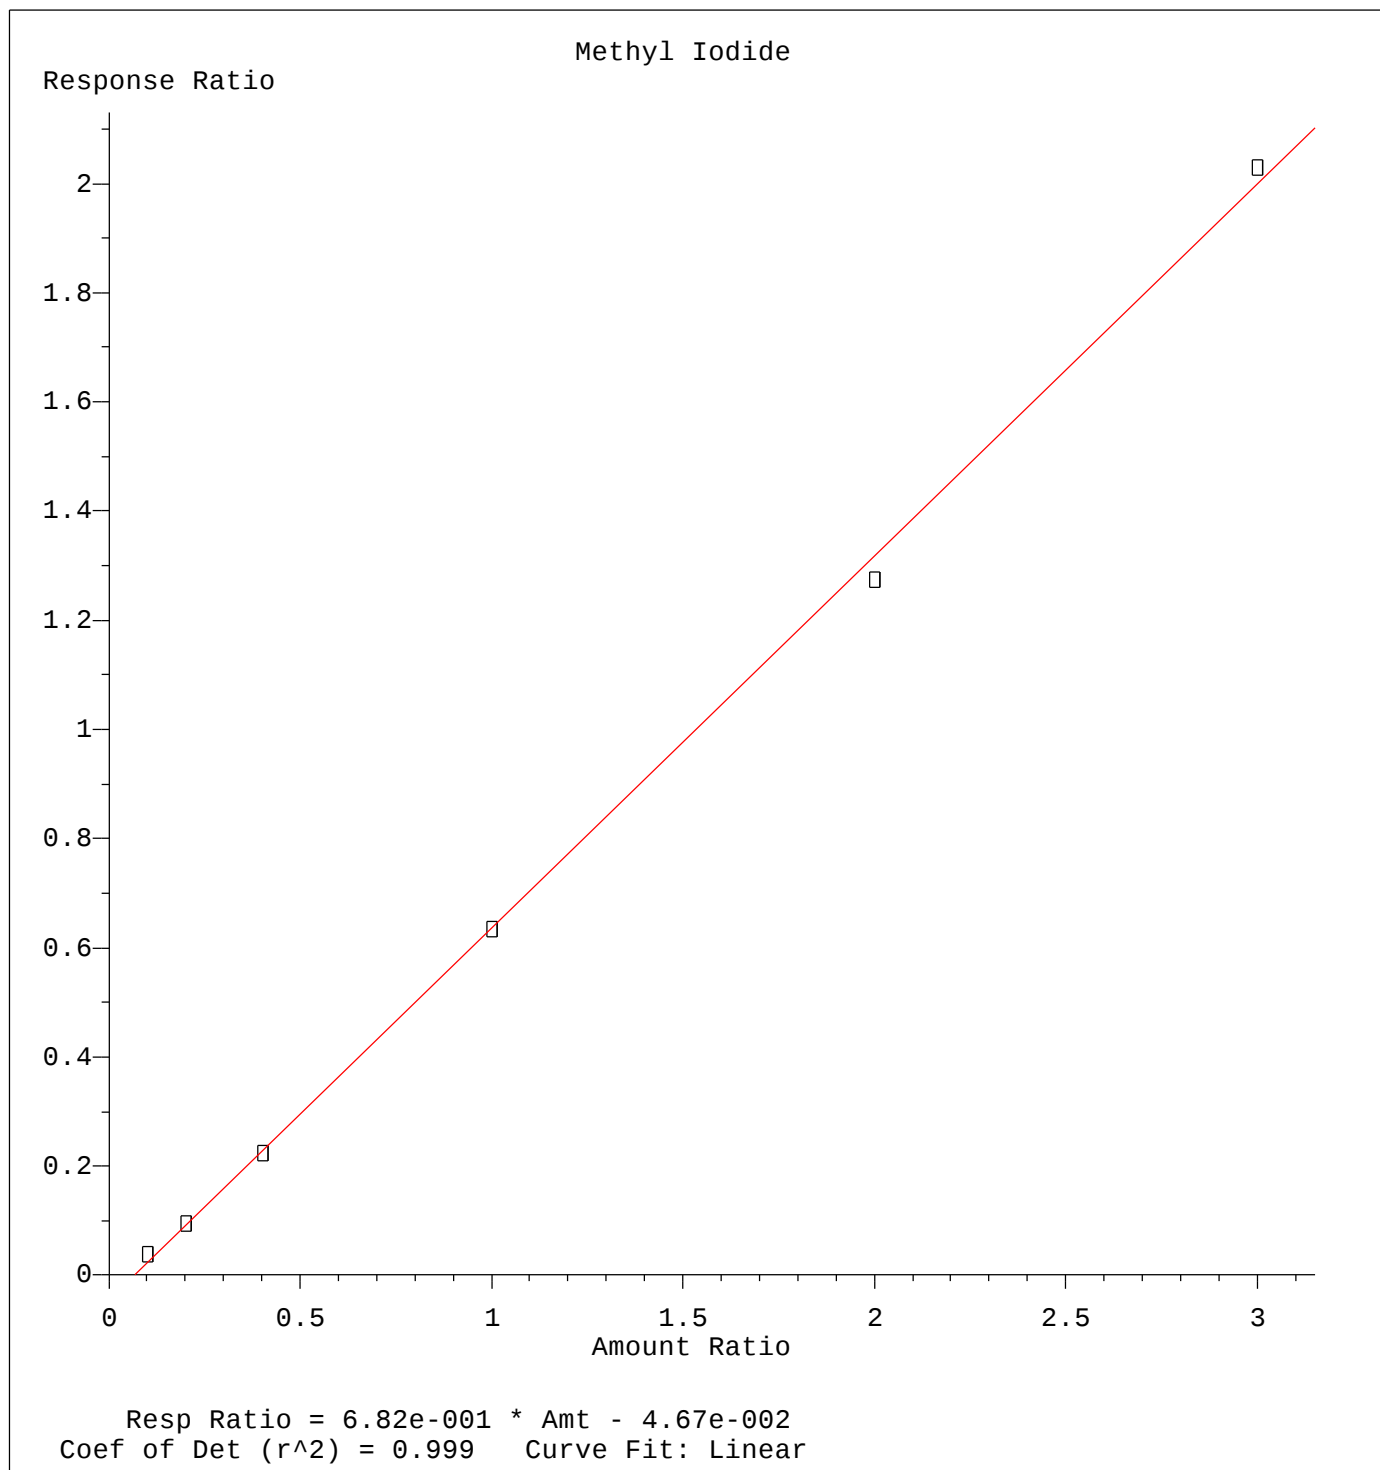

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
Calibration Table Last Updated: Mon Nov 19 16:28:01 2018

Methylene Chloride

Response Ratio

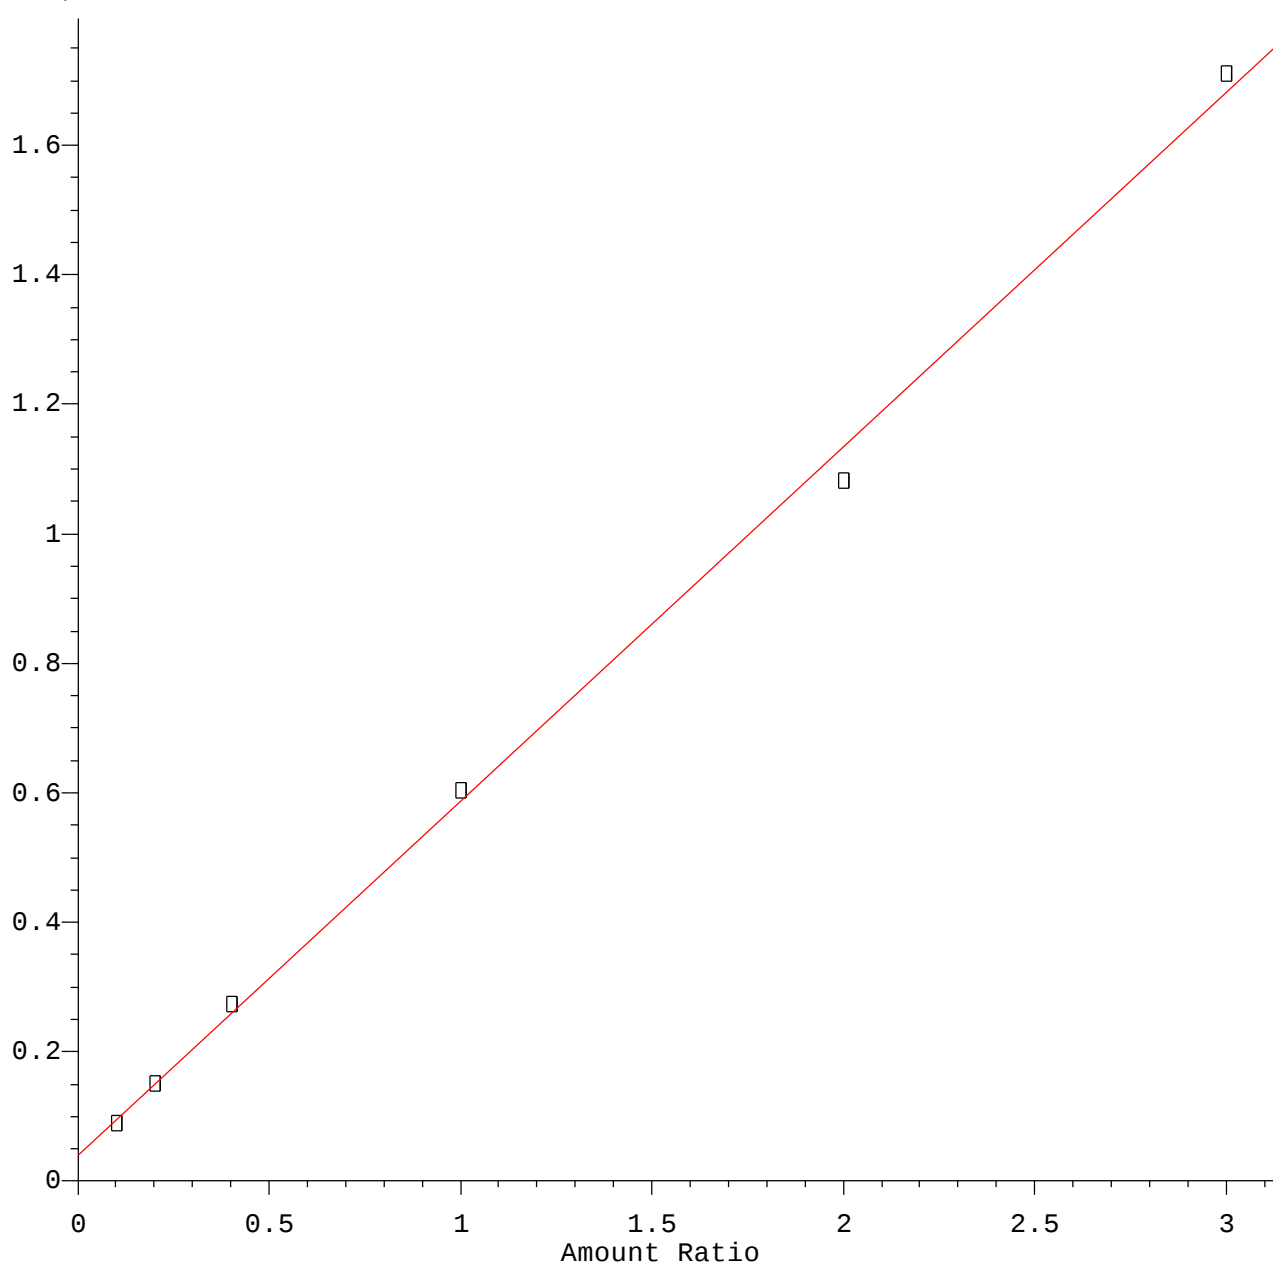

Resp Ratio = $5.47 \times 10^{-1} \times \text{Amt} + 3.96 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
Calibration Table Last Updated: Mon Nov 19 16:28:01 2018