


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111718\
Data File : VW006928.D
Acq On : 16 Nov 2018 22:02
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
Title : SW846 8260
Last Update : Sat Nov 17 04:45:18 2018

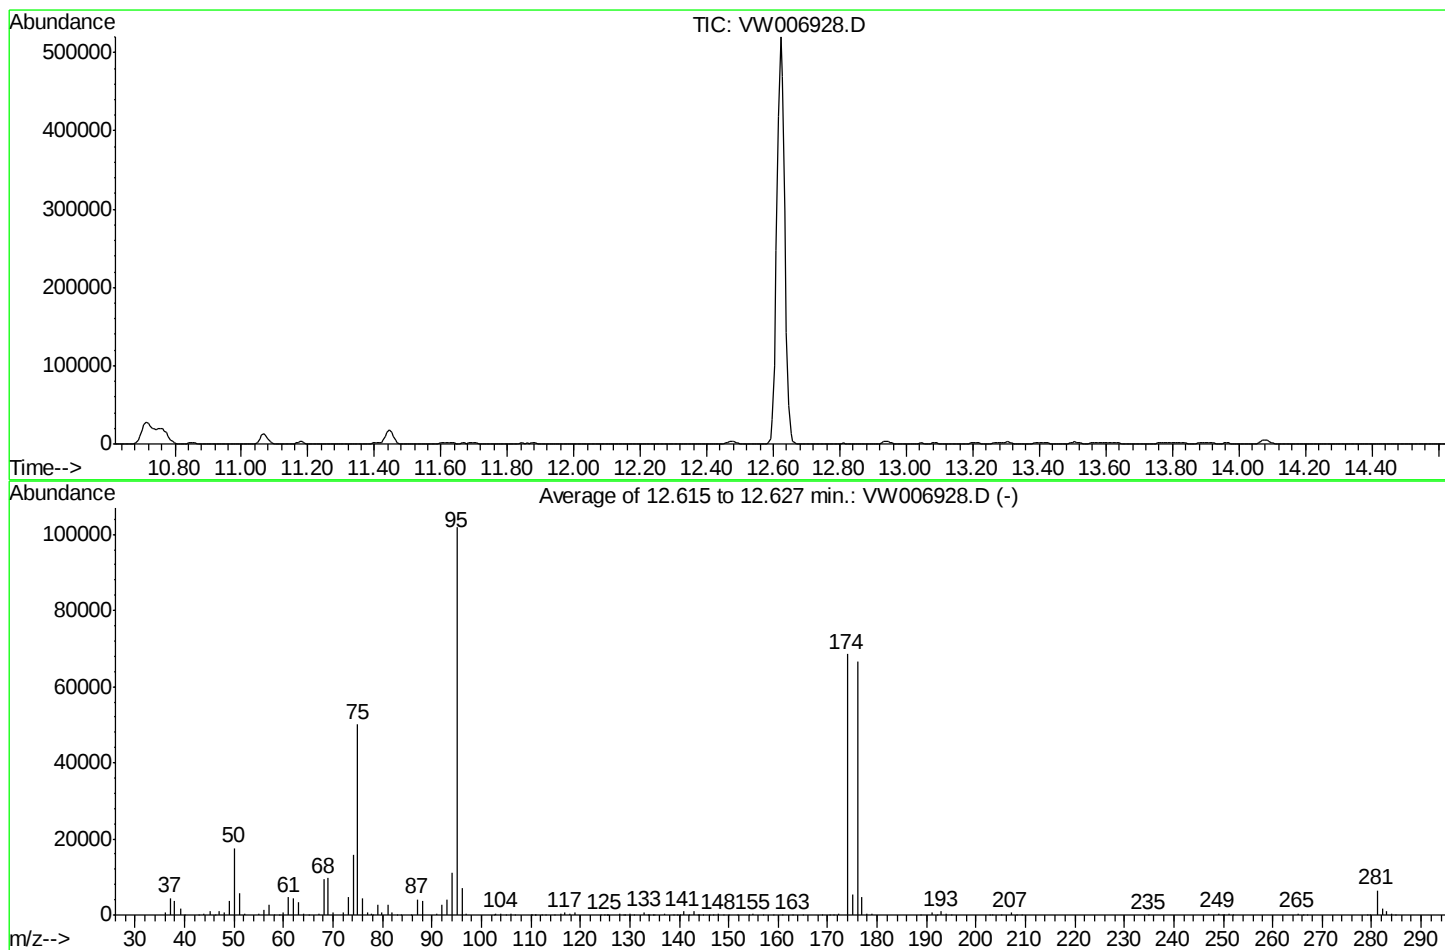

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	17515	PASS
75	95	30	60	49.1	50037	PASS
95	95	100	100	100.0	101861	PASS
96	95	5	9	6.8	6958	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.3	68576	PASS
175	174	5	9	7.9	5446	PASS
176	174	95	101	97.3	66733	PASS
177	176	5	9	7.1	4715	PASS