



Acrolein

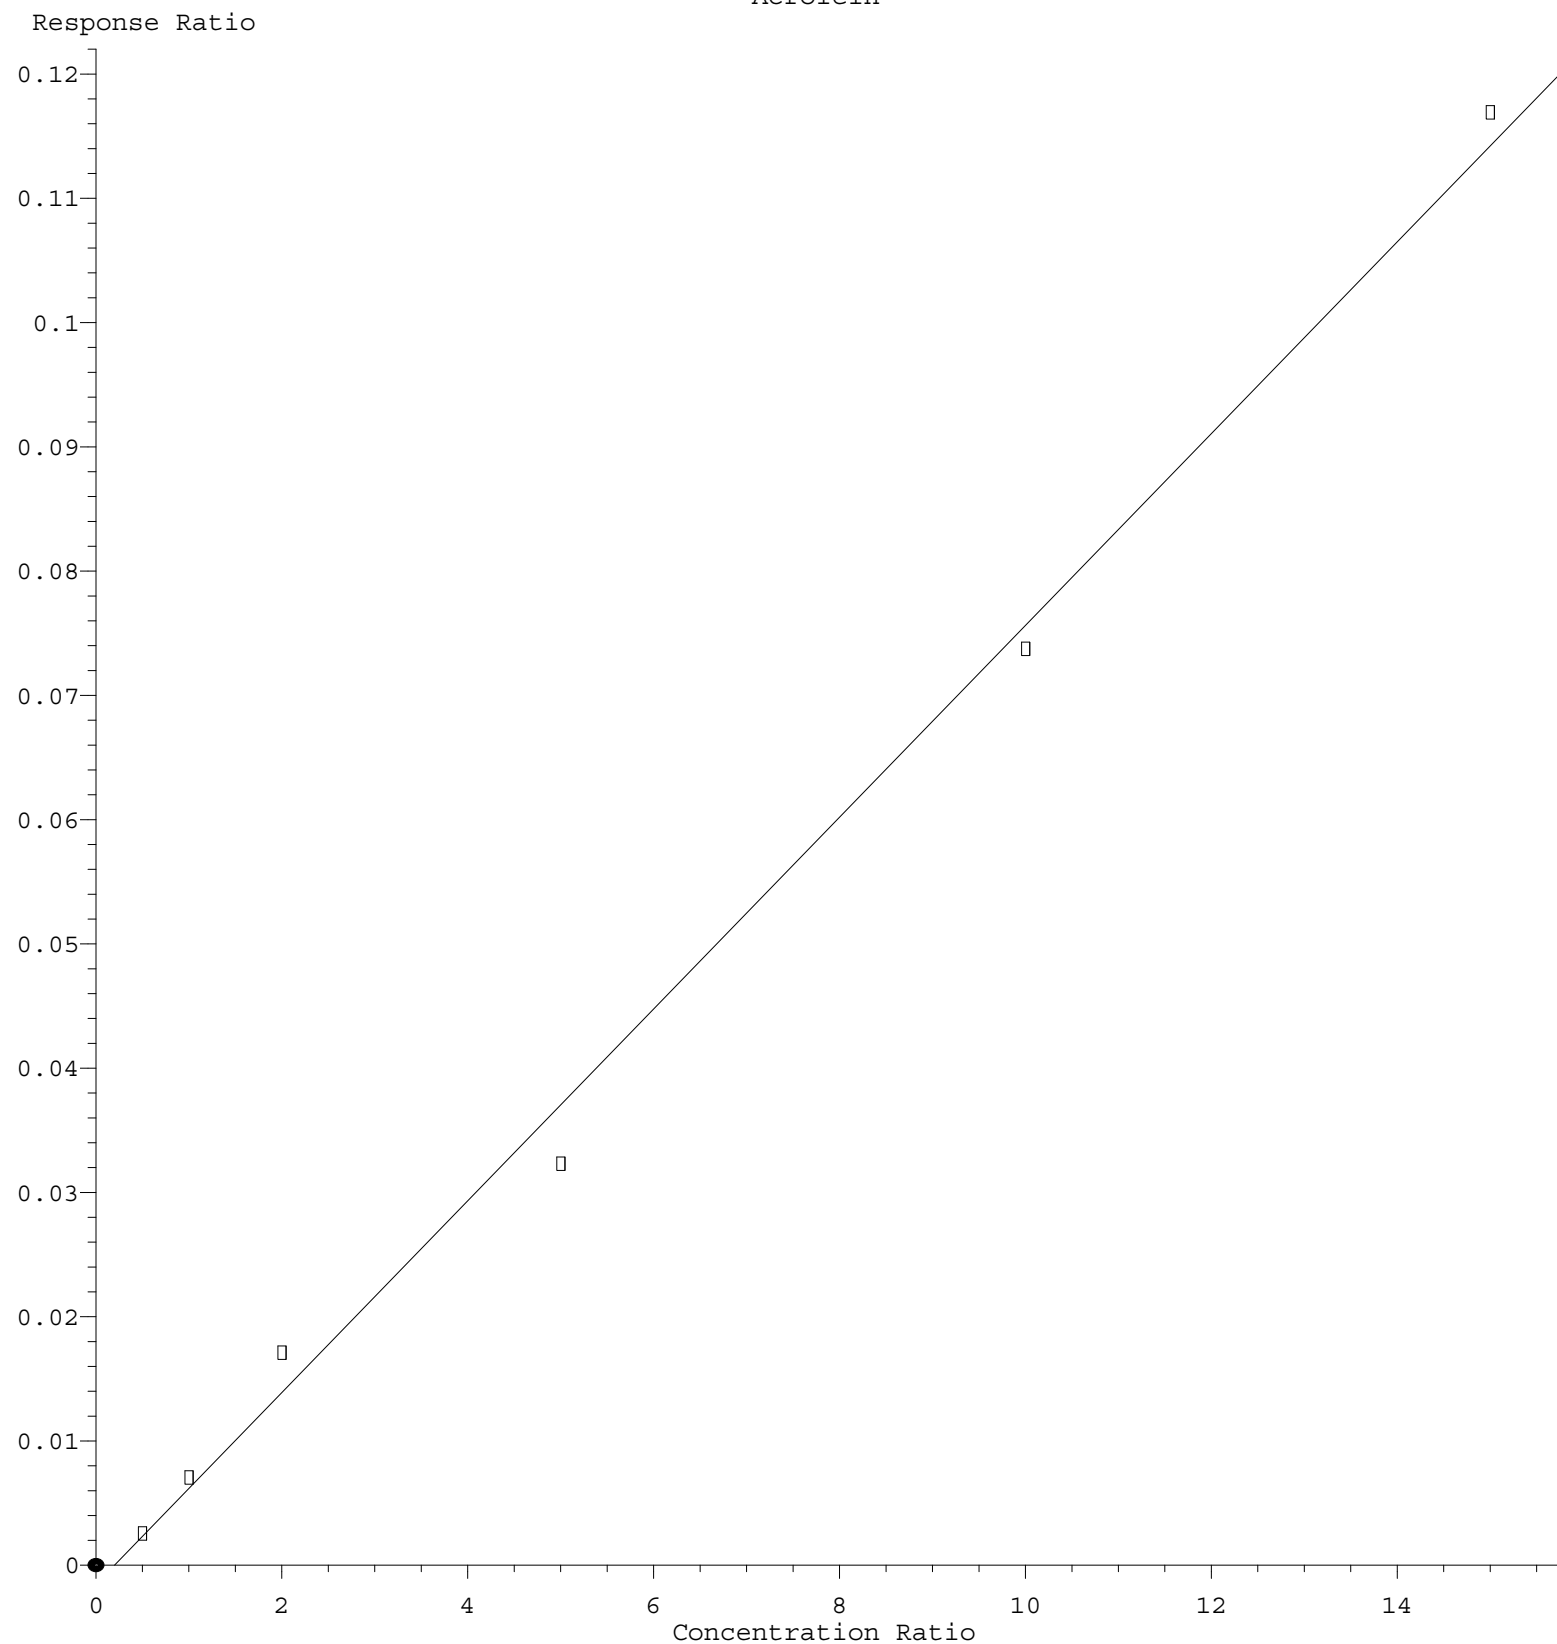

$\text{Response} = 7.736\text{e-}003 * \text{Amt} - 1.578\text{e-}003$
 Coef of Det (r^2) = 0.995613 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111721S.M
 Calibration Table Last Updated: Thu Nov 18 05:03:38 2021

Methylene Chloride

Response Ratio

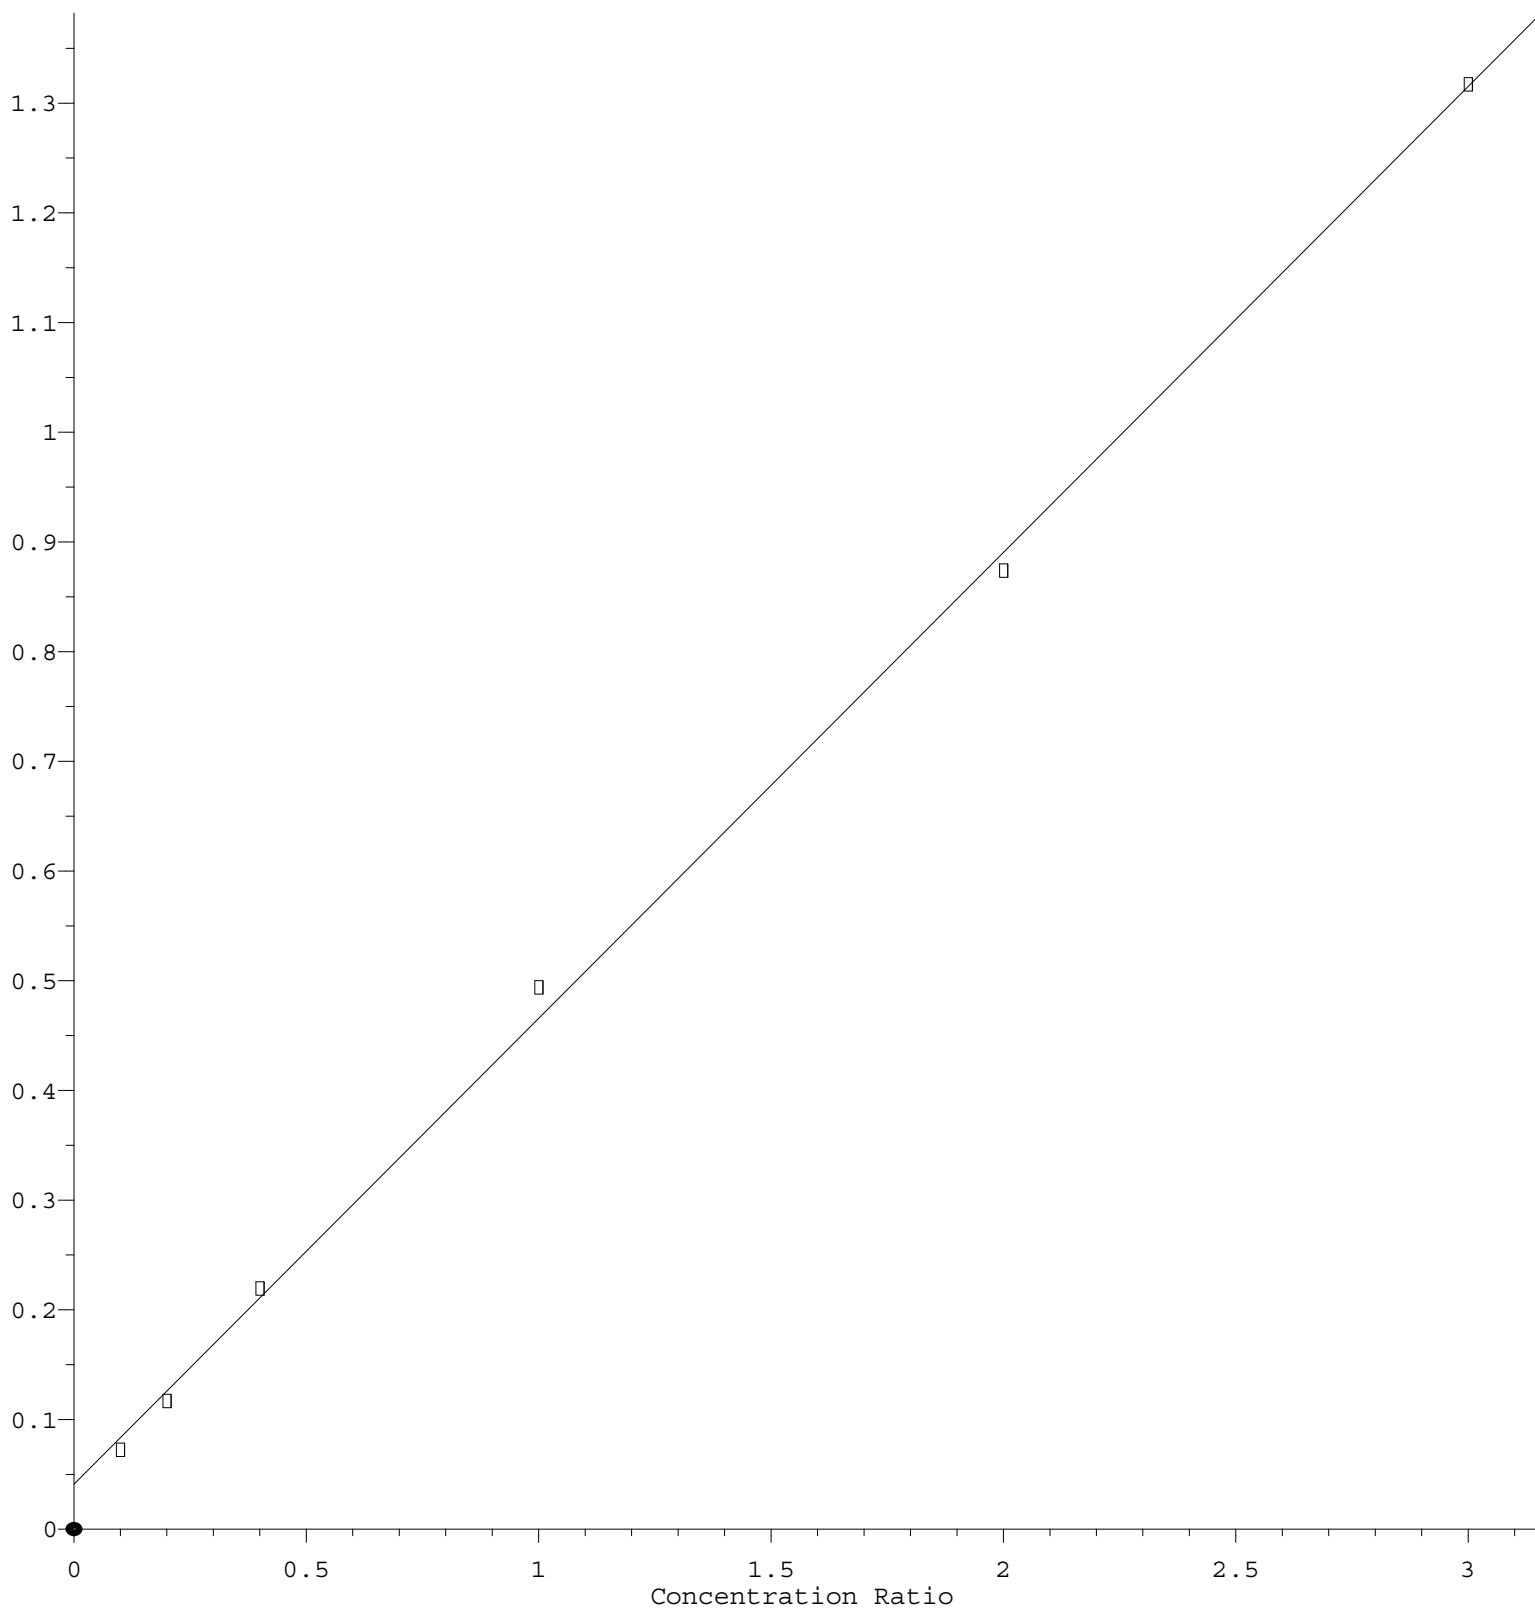

$$\text{Response} = 4.246\text{e-}001 * \text{Amt} + 4.142\text{e-}002$$


Coef of Det (r^2) = 0.998891 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111721S.M

Calibration Table Last Updated: Thu Nov 18 05:03:38 2021

Dichlorodifluoromethane

Response Ratio

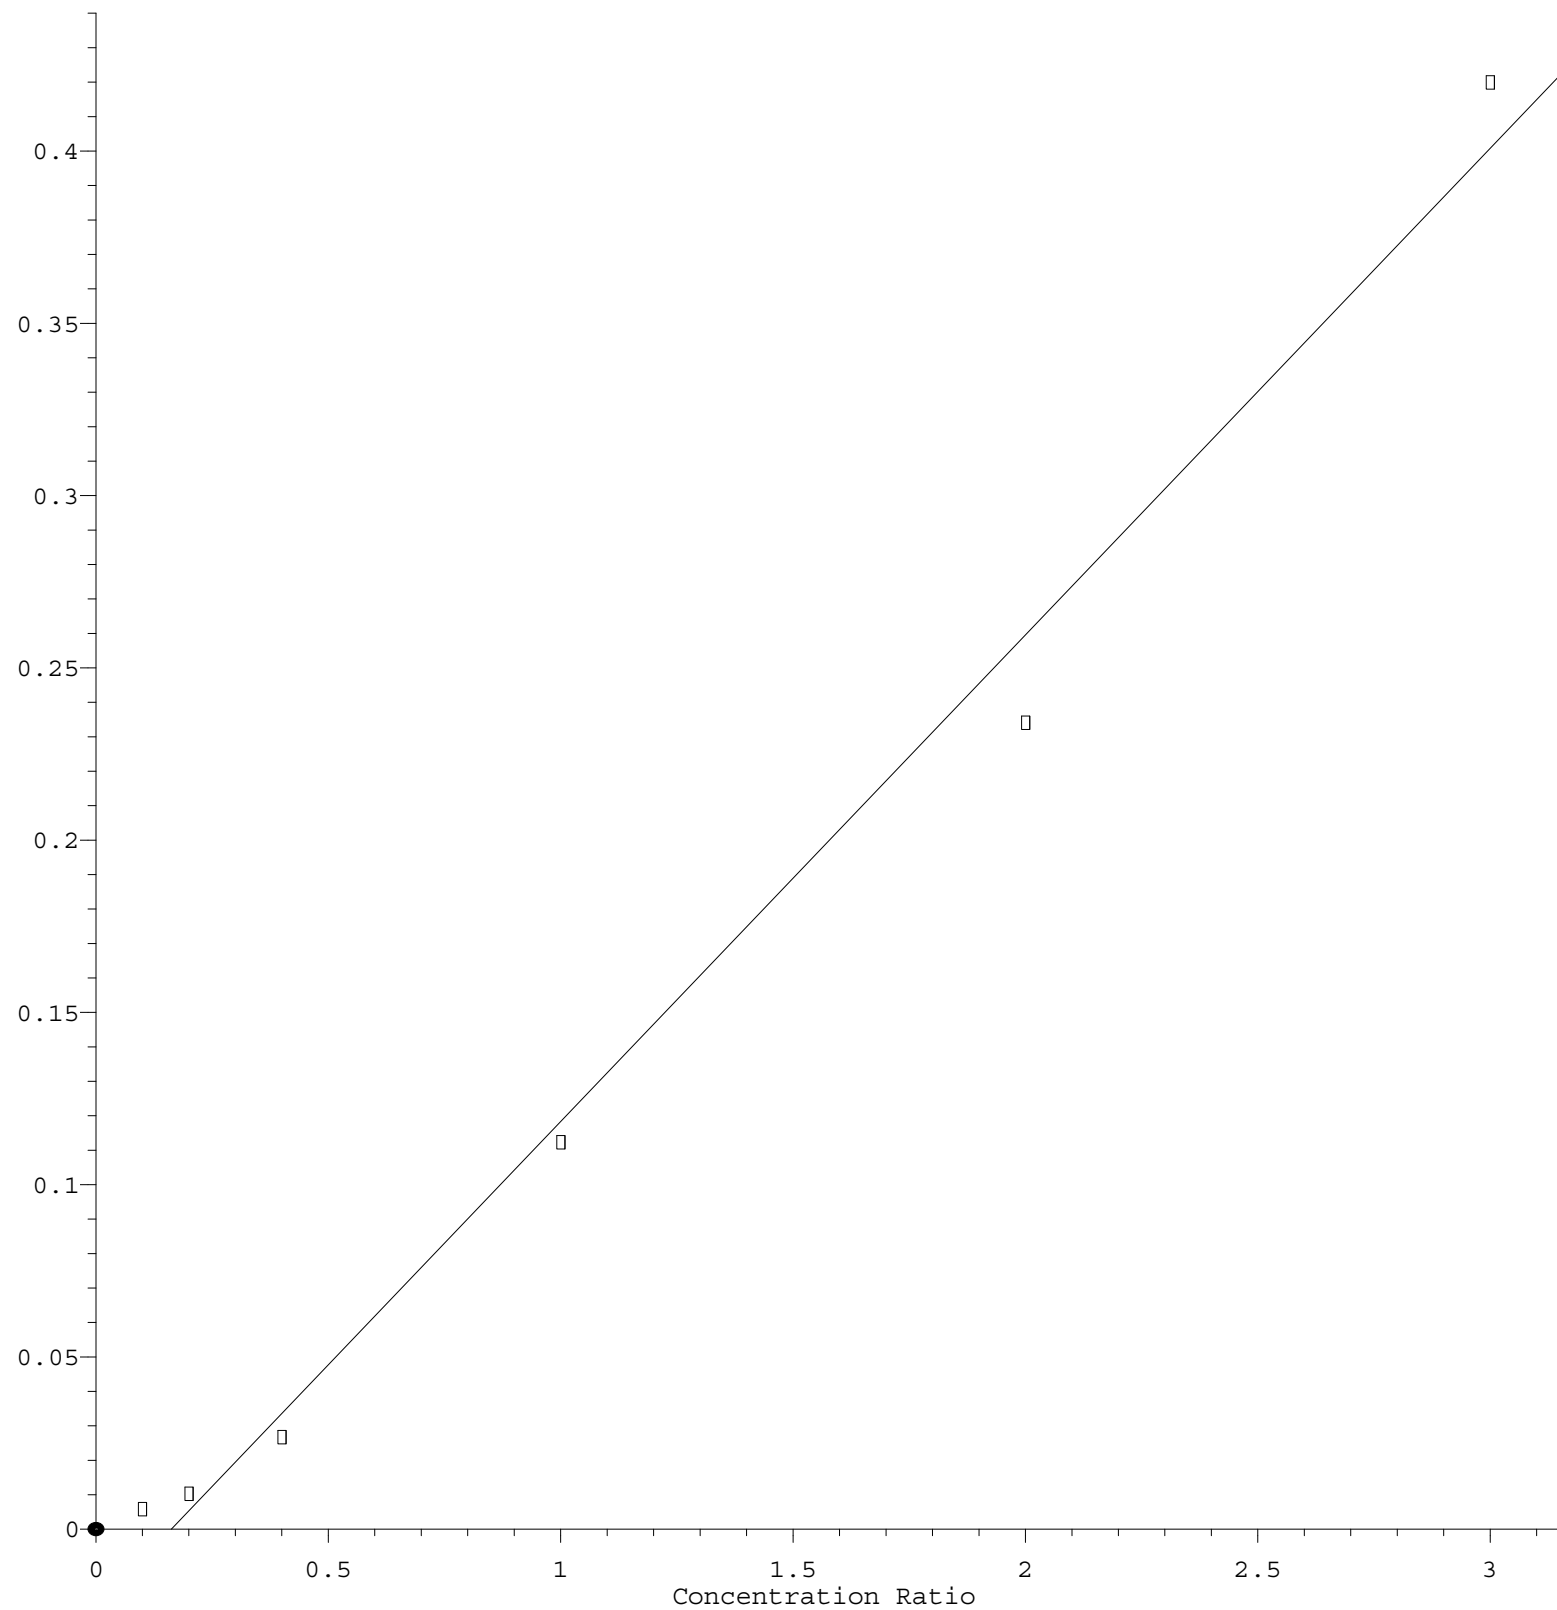

$$\text{Response} = 1.412\text{e-}001 * \text{Amt} - 2.283\text{e-}002$$

Coef of Det (r^2) = 0.990128 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W111721S.M

Calibration Table Last Updated: Thu Nov 18 05:03:38 2021