
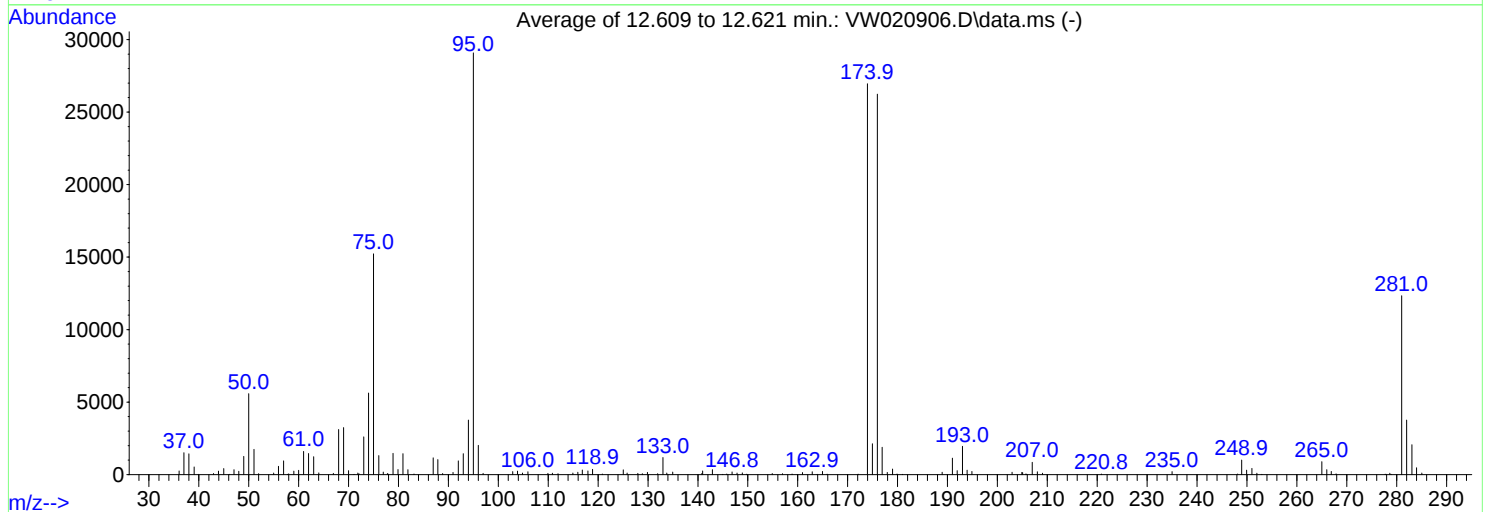


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111721\
 Data File : VW020906.D
 Acq On : 17 Nov 2021 14:51
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111721S.M
 Title : SW846 8260
 Last Update : Thu Nov 18 05:03:38 2021

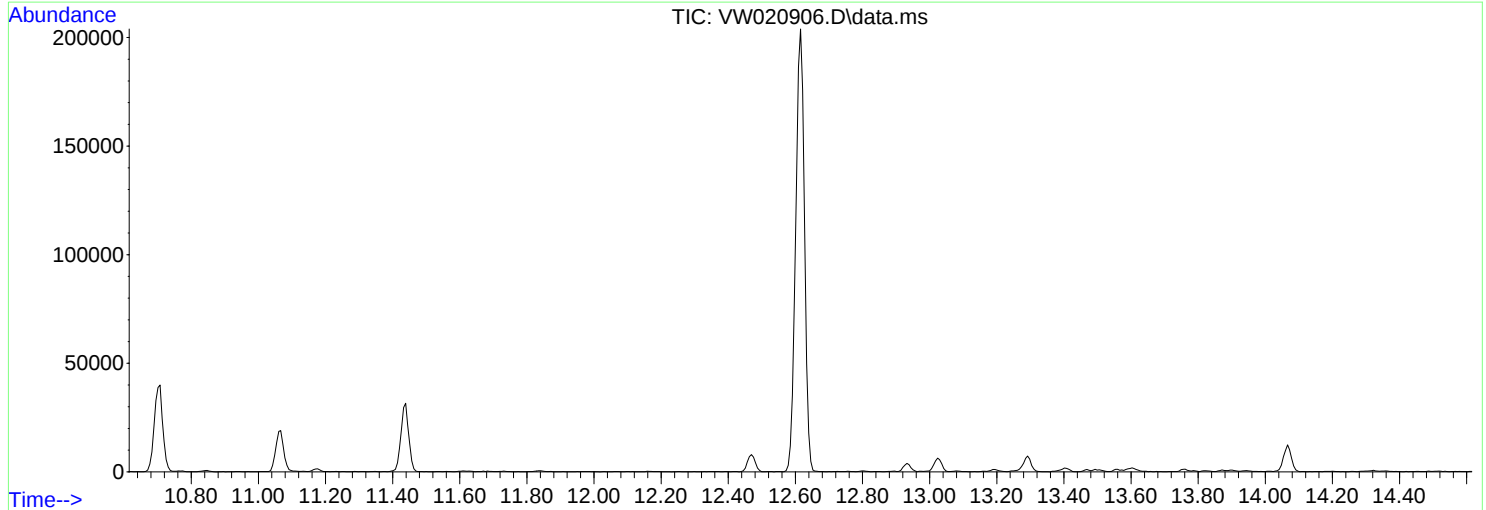

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	5587	PASS
75	95	30	60	52.4	15231	PASS
95	95	100	100	100.0	29085	PASS
96	95	5	9	7.0	2024	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.7	26949	PASS
175	174	5	9	7.9	2133	PASS
176	174	95	101	97.4	26237	PASS
177	176	5	9	7.2	1889	PASS