

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111722\
 Data File : VW025080.D
 Acq On : 17 Nov 2022 16:41
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK588

Quant Time: Nov 18 00:01:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	416488	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	374015	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	180147	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	93294	19.957	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.840%		
7) Chloroethane-d5	2.891	69	74151	27.077	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	108.320%		
11) 1,1-Dichloroethene-d2	4.019	63	168008	14.428	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.720%		
21) 2-Butanone-d5	7.079	46	71664	45.422	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.840%		
24) Chloroform-d	7.652	84	275796	21.820	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.280%		
26) 1,2-Dichloroethane-d4	8.305	65	142359	20.121	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.480%		
32) Benzene-d6	8.274	84	547051	22.820	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.280%		
36) 1,2-Dichloropropane-d6	9.274	67	170765	24.311	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.240%		
41) Toluene-d8	10.323	98	482868	21.635	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.560%		
43) trans-1,3-Dichloroprop...	10.579	79	61631	19.787	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.160%		
47) 2-Hexanone-d5	10.926	63	55127	45.433	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.860%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	131940	23.525	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	158659	22.918	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.680%		
Target Compounds						Qvalue
16) Methylene chloride	4.927	84	23842	3.224	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111722\
Data File : VW025080.D
Acq On : 17 Nov 2022 16:41
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK588

Quant Time: Nov 18 00:01:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

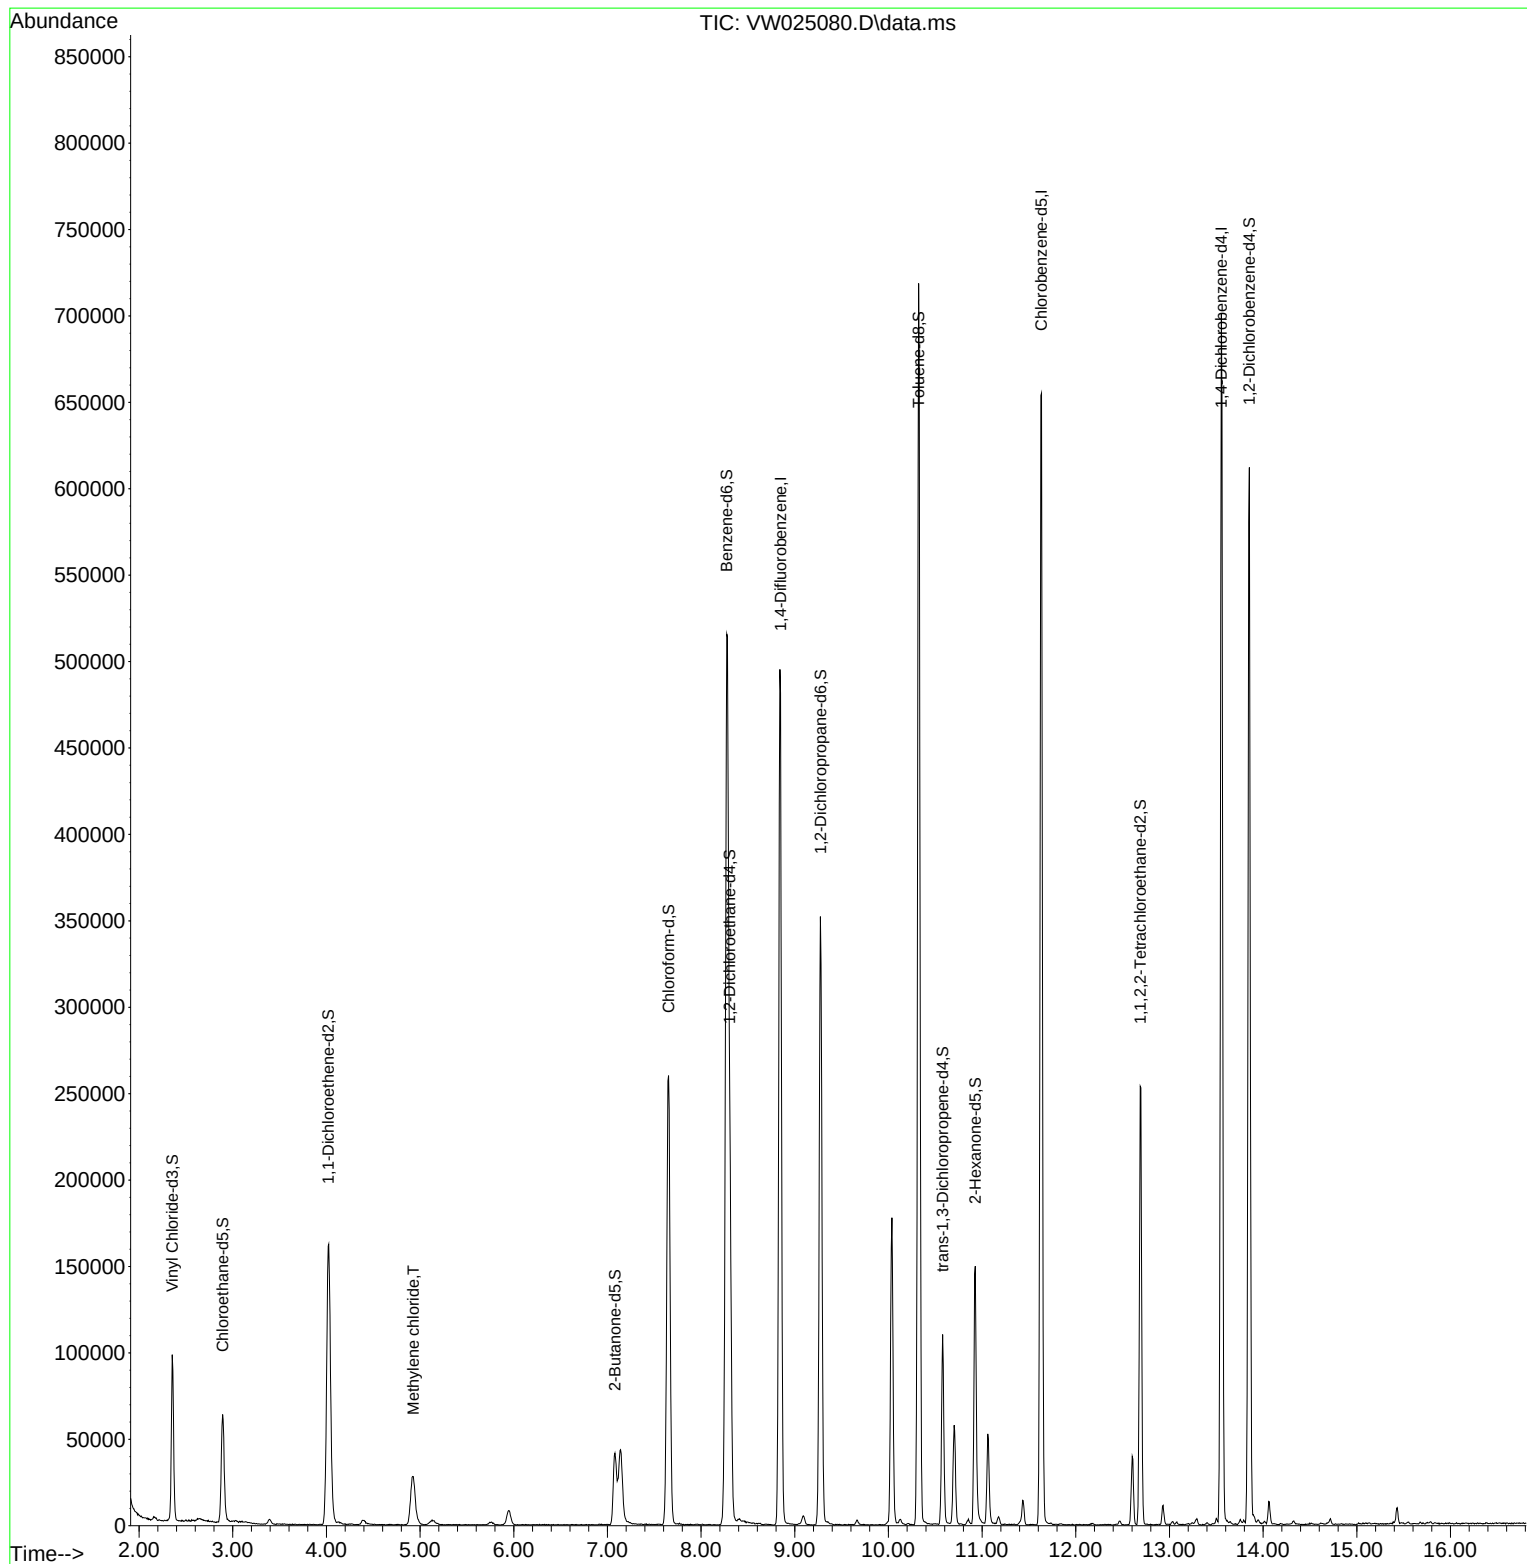

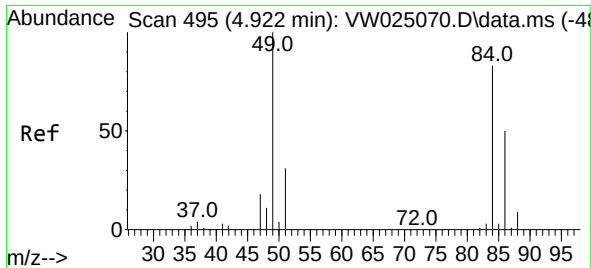

#16
Methylene chloride
Concen: 3.224 ug/L
RT: 4.927 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW025080.D
Acq: 17 Nov 2022 16:41

Instrument :
MSVOA_W
ClientSampleId :
VIBLK588

Tgt Ion: 84 Resp: 23842

Ion	Ratio	Lower	Upper
84	100		
86	57.4	42.6	79.0
49	110.5	81.9	152.1

