




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111722\
Data File : VW025081.D
Acq On : 17 Nov 2022 17:05
Operator : SY/VA
Sample : N5679-04RE
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0KZ6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2022
Supervised By :Mahesh Dadoda 11/28/2022

Quant Time: Nov 18 00:01:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

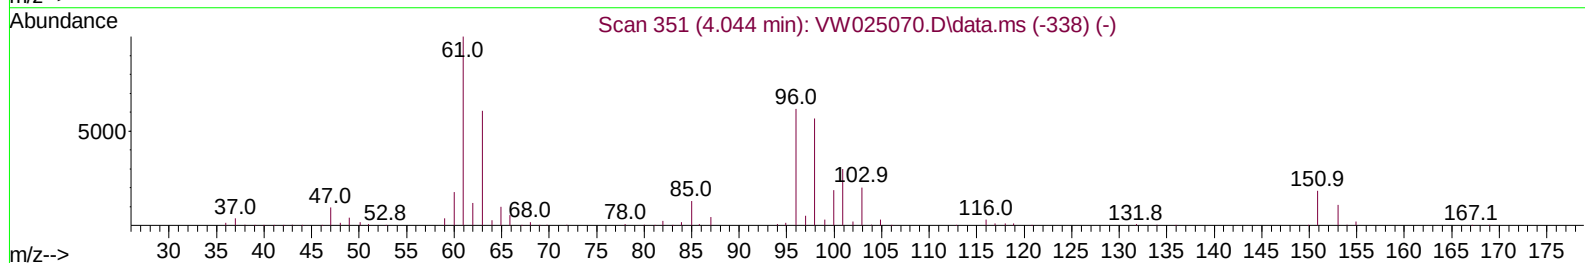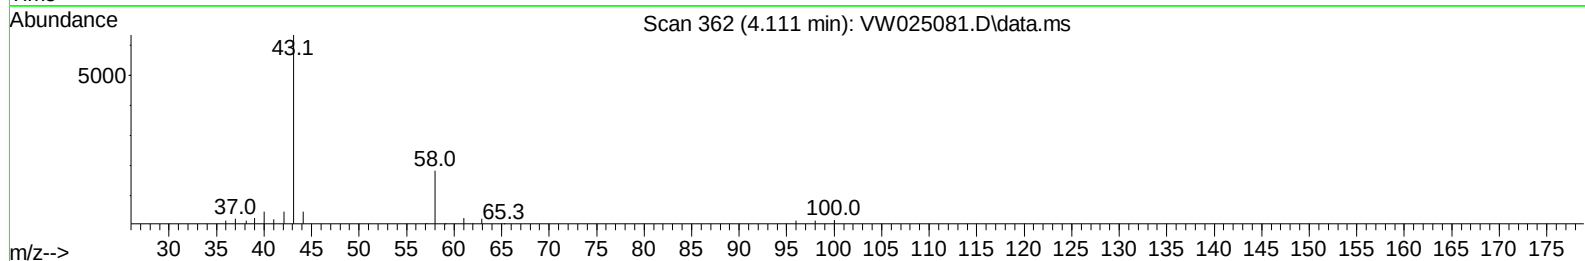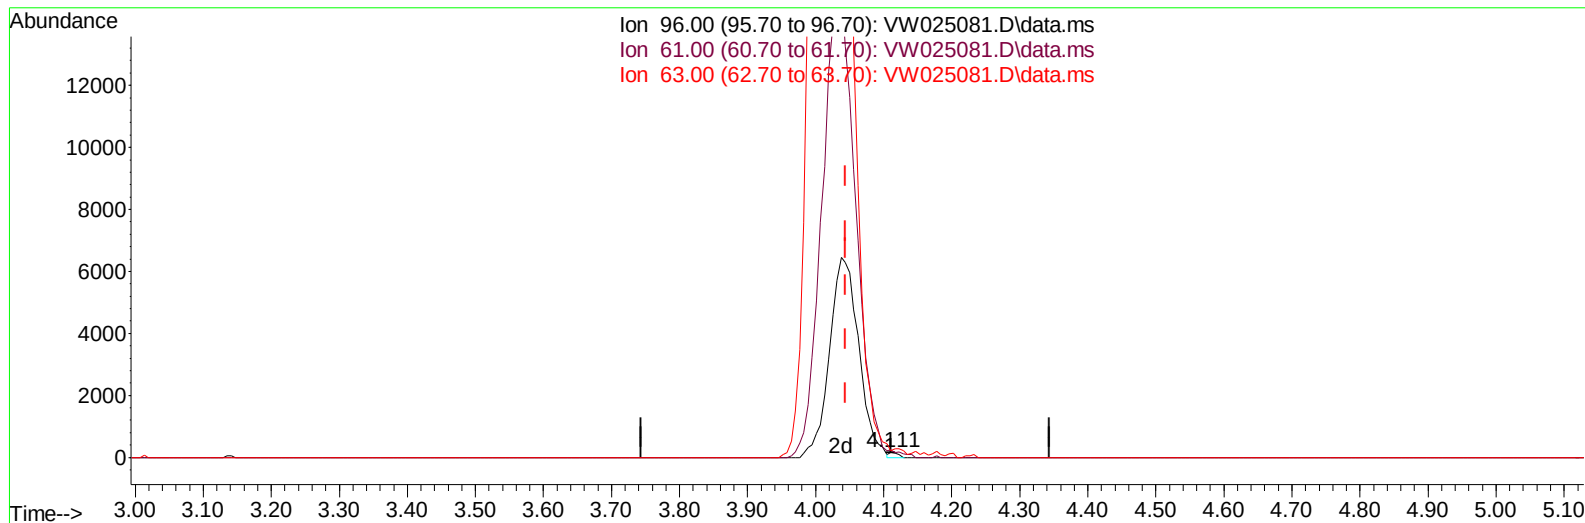

TIC: VW025081.D\data.ms

(12) 1,1-Dichloroethene (T)

4.111min (+ 0.067) 0.03 ug/L

response 142

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	180.30	152.50
63.00	140.50	139.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111722\
 Data File : VW025081.D
 Acq On : 17 Nov 2022 17:05
 Operator : SY/VA
 Sample : N5679-04RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0KZ6

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:01:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/28/2022
 Supervised By :Mahesh Dadoda 11/28/2022

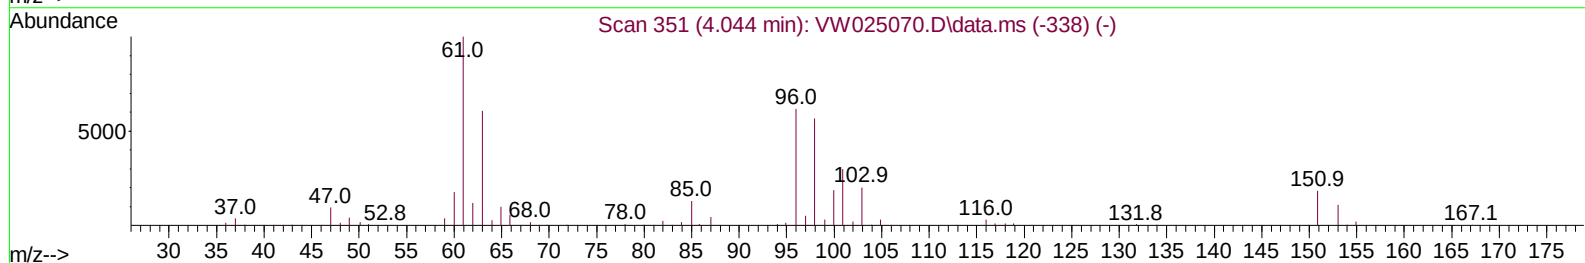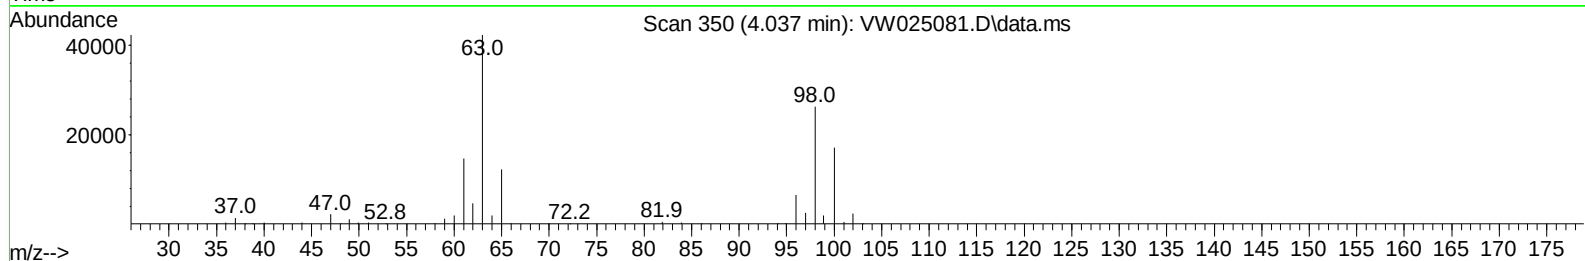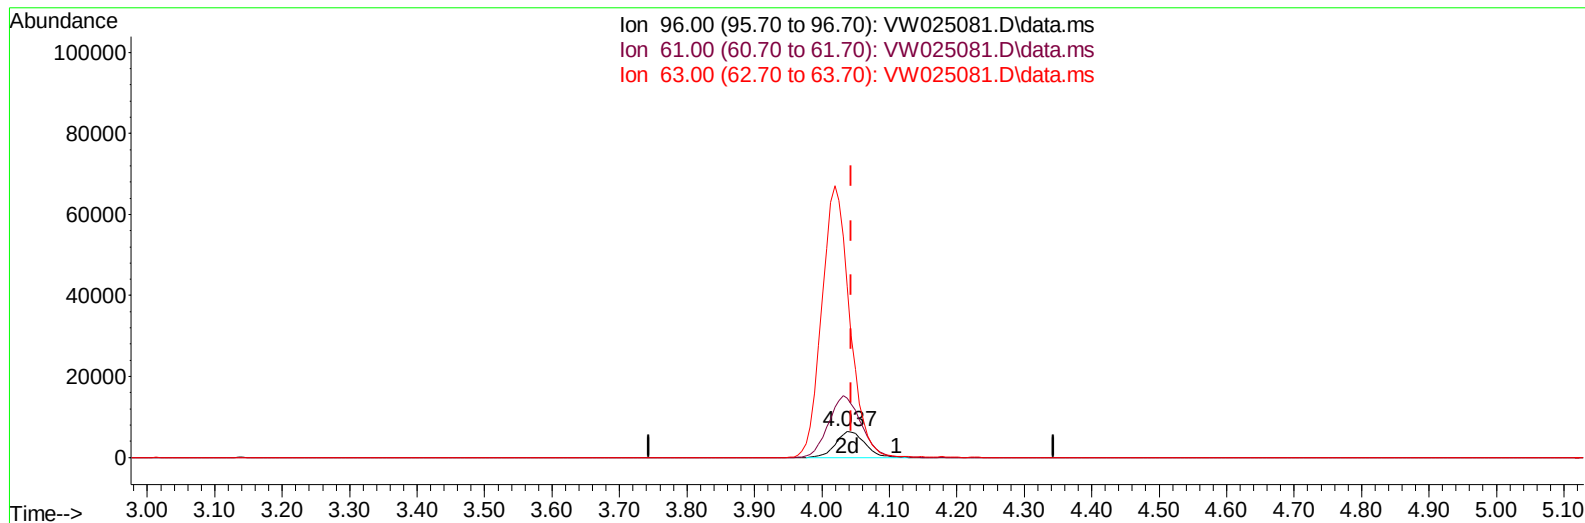

TIC: VW025081.D\data.ms

(12) 1,1-Dichloroethene (T)

4.037min (-0.006) 3.45 ug/L m

response 19402

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	180.30	227.20
63.00	140.50	654.96#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw111722\
 Data File : VW025081.D
 Acq On : 17 Nov 2022 17:05
 Operator : SY/VA
 Sample : N5679-04RE
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COKZ6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2022
 Supervised By :Mahesh Dadoda 11/28/2022

Quant Time: Nov 18 00:01:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	453110	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	390026	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155267	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	96708	19.015	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.080%	
7) Chloroethane-d5	2.885	69	76707	25.747	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	4.019	63	192813	15.220	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.880%	
21) 2-Butanone-d5	7.080	46	95851	55.842	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.680%	
24) Chloroform-d	7.653	84	316539	23.019	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.080%	
26) 1,2-Dichloroethane-d4	8.305	65	162750	21.144	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	84.560%	
32) Benzene-d6	8.275	84	613344	24.535	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	98.120%	
36) 1,2-Dichloropropane-d6	9.274	67	192836	26.326	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.320%	
41) Toluene-d8	10.323	98	537915	23.112	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	92.440%	
43) trans-1,3-Dichloroprop...	10.579	79	73129	22.515	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.040%	
47) 2-Hexanone-d5	10.920	63	66668	52.689	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	105.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	152635	26.097	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	13.853	152	136108	22.811	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.240%	
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	4.037	96	19402m	3.452	ug/L	
13) Acetone	4.129	43	27468	22.526	ug/L	100
14) Carbon disulfide	4.385	76	26306	1.602	ug/L	100
19) 1,1-Dichloroethane	6.214	63	19783	1.775	ug/L	95
20) cis-1,2-Dichloroethene	7.177	96	21622	3.296	ug/L	98
34) Trichloroethene	9.091	95	1463333	235.356	ug/L	97
46) Tetrachloroethene	10.859	164	165671	37.258	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111722\
Data File : VW025081.D
Acq On : 17 Nov 2022 17:05
Operator : SY/VA
Sample : N5679-04RE
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0KZ6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2022
Supervised By :Mahesh Dadoda 11/28/2022

Quant Time: Nov 18 00:01:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

