

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111819\
 Data File : VW014060.D
 Acq On : 18 Nov 2019 14:28
 Operator : SY/VA
 Sample : K5810-06
 Misc : 4.37G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFLQ8

Manual Integrations
 APPROVED

MMDadoda
 11/20/2019 3:02:31 AM

Quant Time: Nov 19 07:55:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 19 07:22:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	343787	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	335370	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	186001	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	112688	20.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.20%
7) Chloroethane-d5	2.89	69	101191	22.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.04%
10) 1,1-Dichloroethene-d2	4.02	63	187847	16.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.76%
20) 2-Butanone-d5	7.07	46	90036	56.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.00%
24) Chloroform-d	7.65	84	270307	25.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.28%
26) 1,2-Dichloroethane-d4	8.31	65	147619	27.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.12%
29) Benzene-d6	8.27	84	569796	23.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.80%
33) 1,2-Dichloropropane-d6	9.27	67	174430	25.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.08%
37) Toluene-d8	10.32	98	529700	23.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.88%
38) trans-1,3-Dichloropropene-	10.58	79	75078	25.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.60%
39) 2-Hexanone-d5	10.92	63	70067	53.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	145567	27.66	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.64%
61) 1,2-Dichlorobenzene-d4	13.85	152	191625	25.64	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.56%

Target Compounds				Ovalue
13) Acetone	4.12	43	4238m	2.614 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111819\
Data File : VW014060.D
Acq On : 18 Nov 2019 14:28
Operator : SY/VA
Sample : K5810-06
Misc : 4.37G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFLQ8

Manual Integrations
APPROVED

MMDadoda
11/20/2019 3:02:31 AM

Quant Time: Nov 19 07:55:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 19 07:22:02 2019
Response via : Initial Calibration

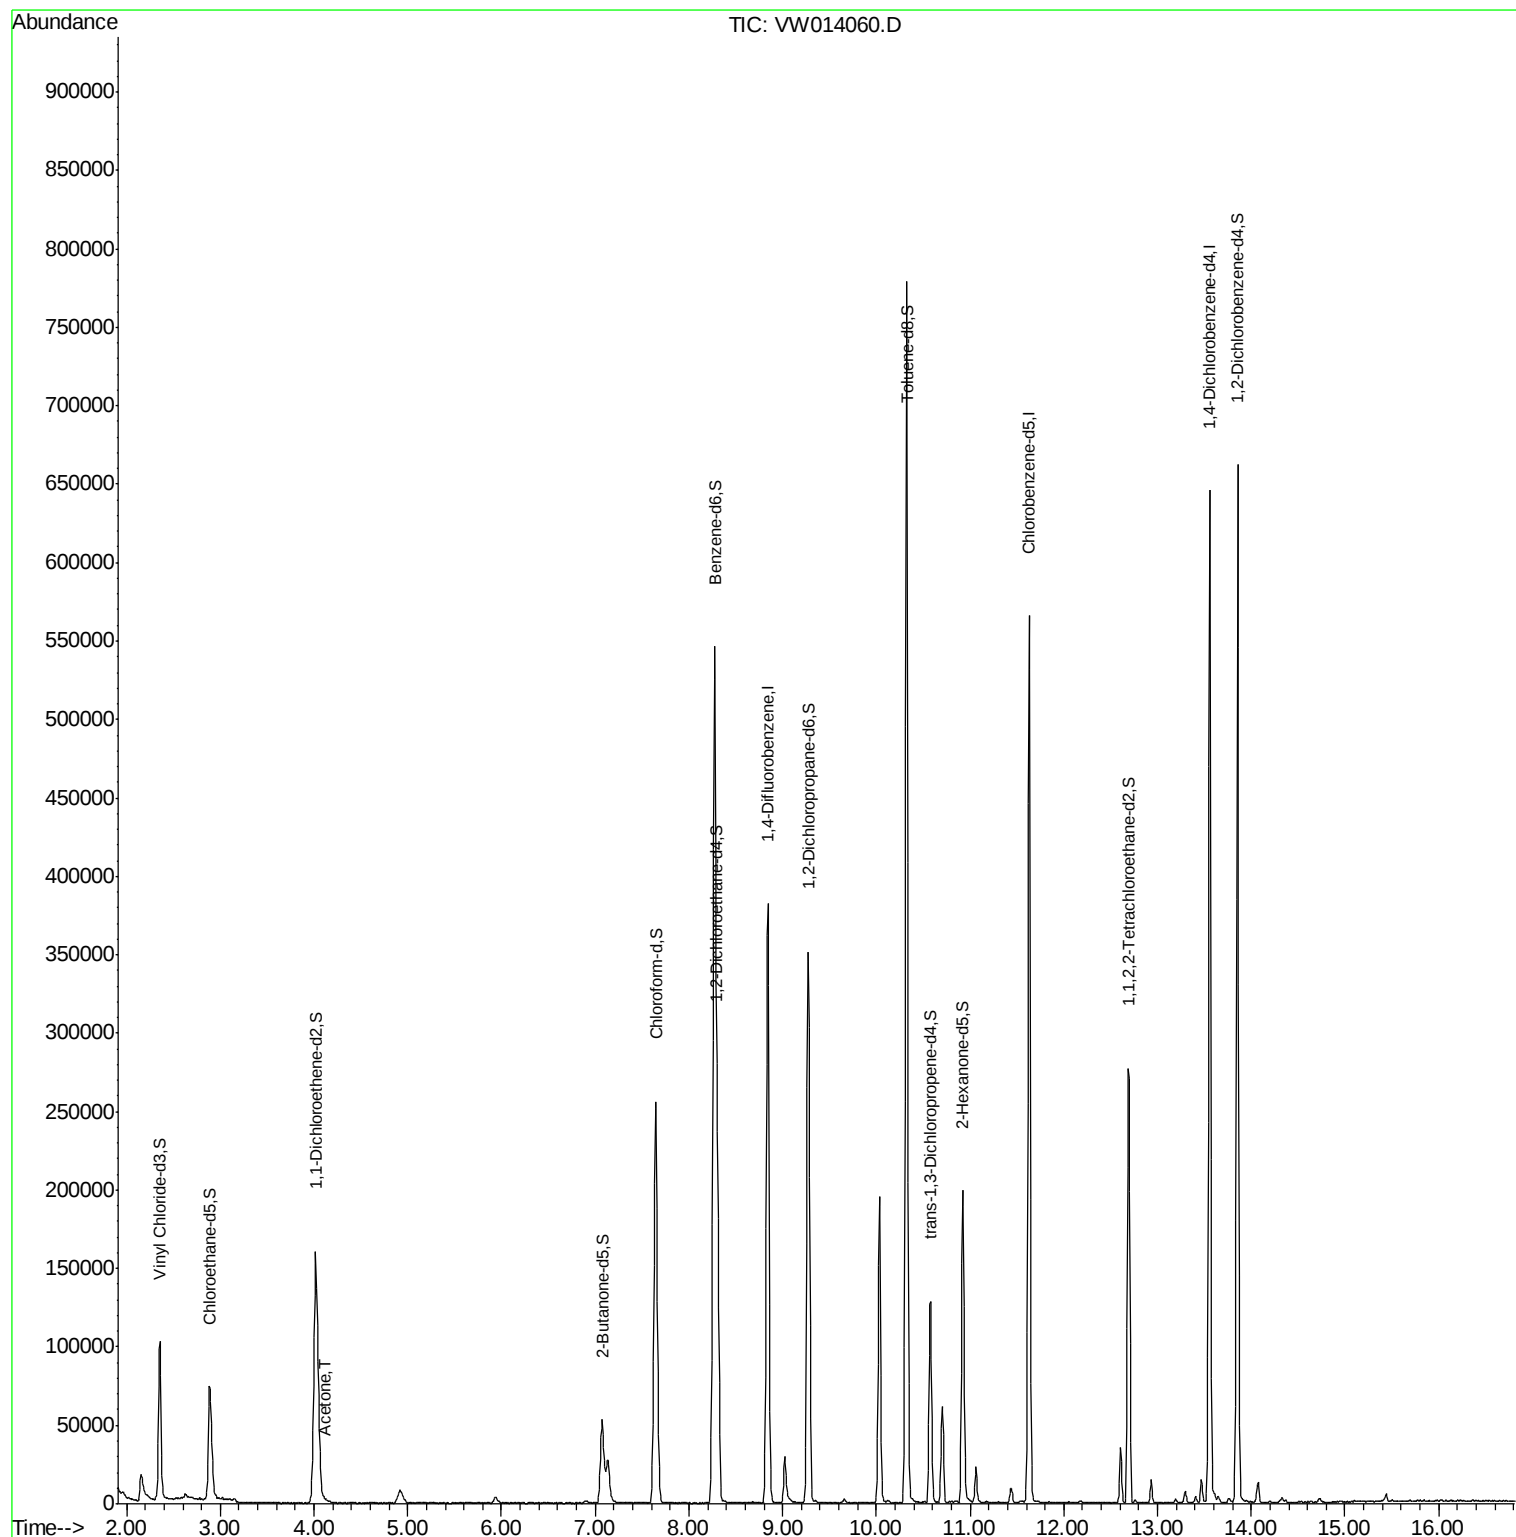

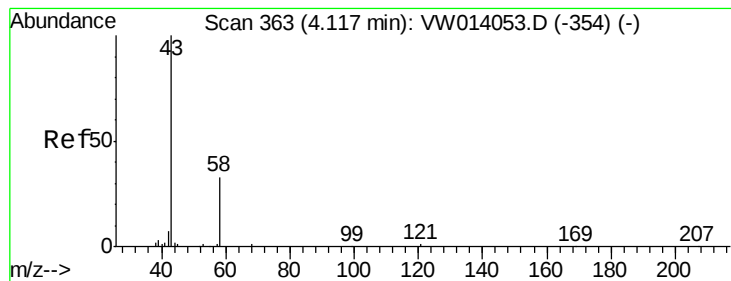

#13
 Acetone
 Concen: 2.614 ug/L m
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW014060.D
 Acq: 18 Nov 2019 14:28

Instrument :
 MSVOA_W
 ClientSampled :
 BFLQ8

Tot Ion	Ratio	Lower	Upper
43	100		
58	15.7	0.0	65.4

Manual Integrations
 APPROVED

MMDadoda
 11/20/2019 3:02:31 AM

