

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111820\
 Data File : VW017325.D
 Acq On : 18 Nov 2020 13:47
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Quant Time: Nov 18 15:31:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 18 15:21:54 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	405201	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	366417	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	184598	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.36	65	139812	23.31	ug/L	0.00
7) Chloroethane-d5	2.90	69	113111	23.74	ug/L	0.00
10) 1,1-Dichloroethene-d2	4.02	63	190251	18.13	ug/L	0.00
20) 2-Butanone-d5	7.08	46	51103	51.87	ug/L	0.00
24) Chloroform-d	7.65	84	249641	23.45	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.31	65	129882	25.25	ug/L	0.00
29) Benzene-d6	8.27	84	508987	24.64	ug/L	0.00
33) 1,2-Dichloropropane-d6	9.27	67	135924	24.70	ug/L	0.00
37) Toluene-d8	10.32	98	481088	24.74	ug/L	0.00
38) trans-1,3-Dichloropropene-	10.58	79	59268	24.74	ug/L	0.00
39) 2-Hexanone-d5	10.93	63	39951	54.14	ug/L	0.00
48) 1,1,2,2-Tetrachloroethane-	12.69	84	111532	26.75	ug/L	0.00
61) 1,2-Dichlorobenzene-d4	13.85	152	170273	24.99	ug/L	0.00
Target Compounds						
13) Acetone	4.13	43	1812	2.521	ug/L	Qvalue 68
16) Methylene chloride	4.92	84	12658	1.826	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111820\
Data File : VW017325.D
Acq On : 18 Nov 2020 13:47
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Quant Time: Nov 18 15:31:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 18 15:21:54 2020
Response via : Initial Calibration

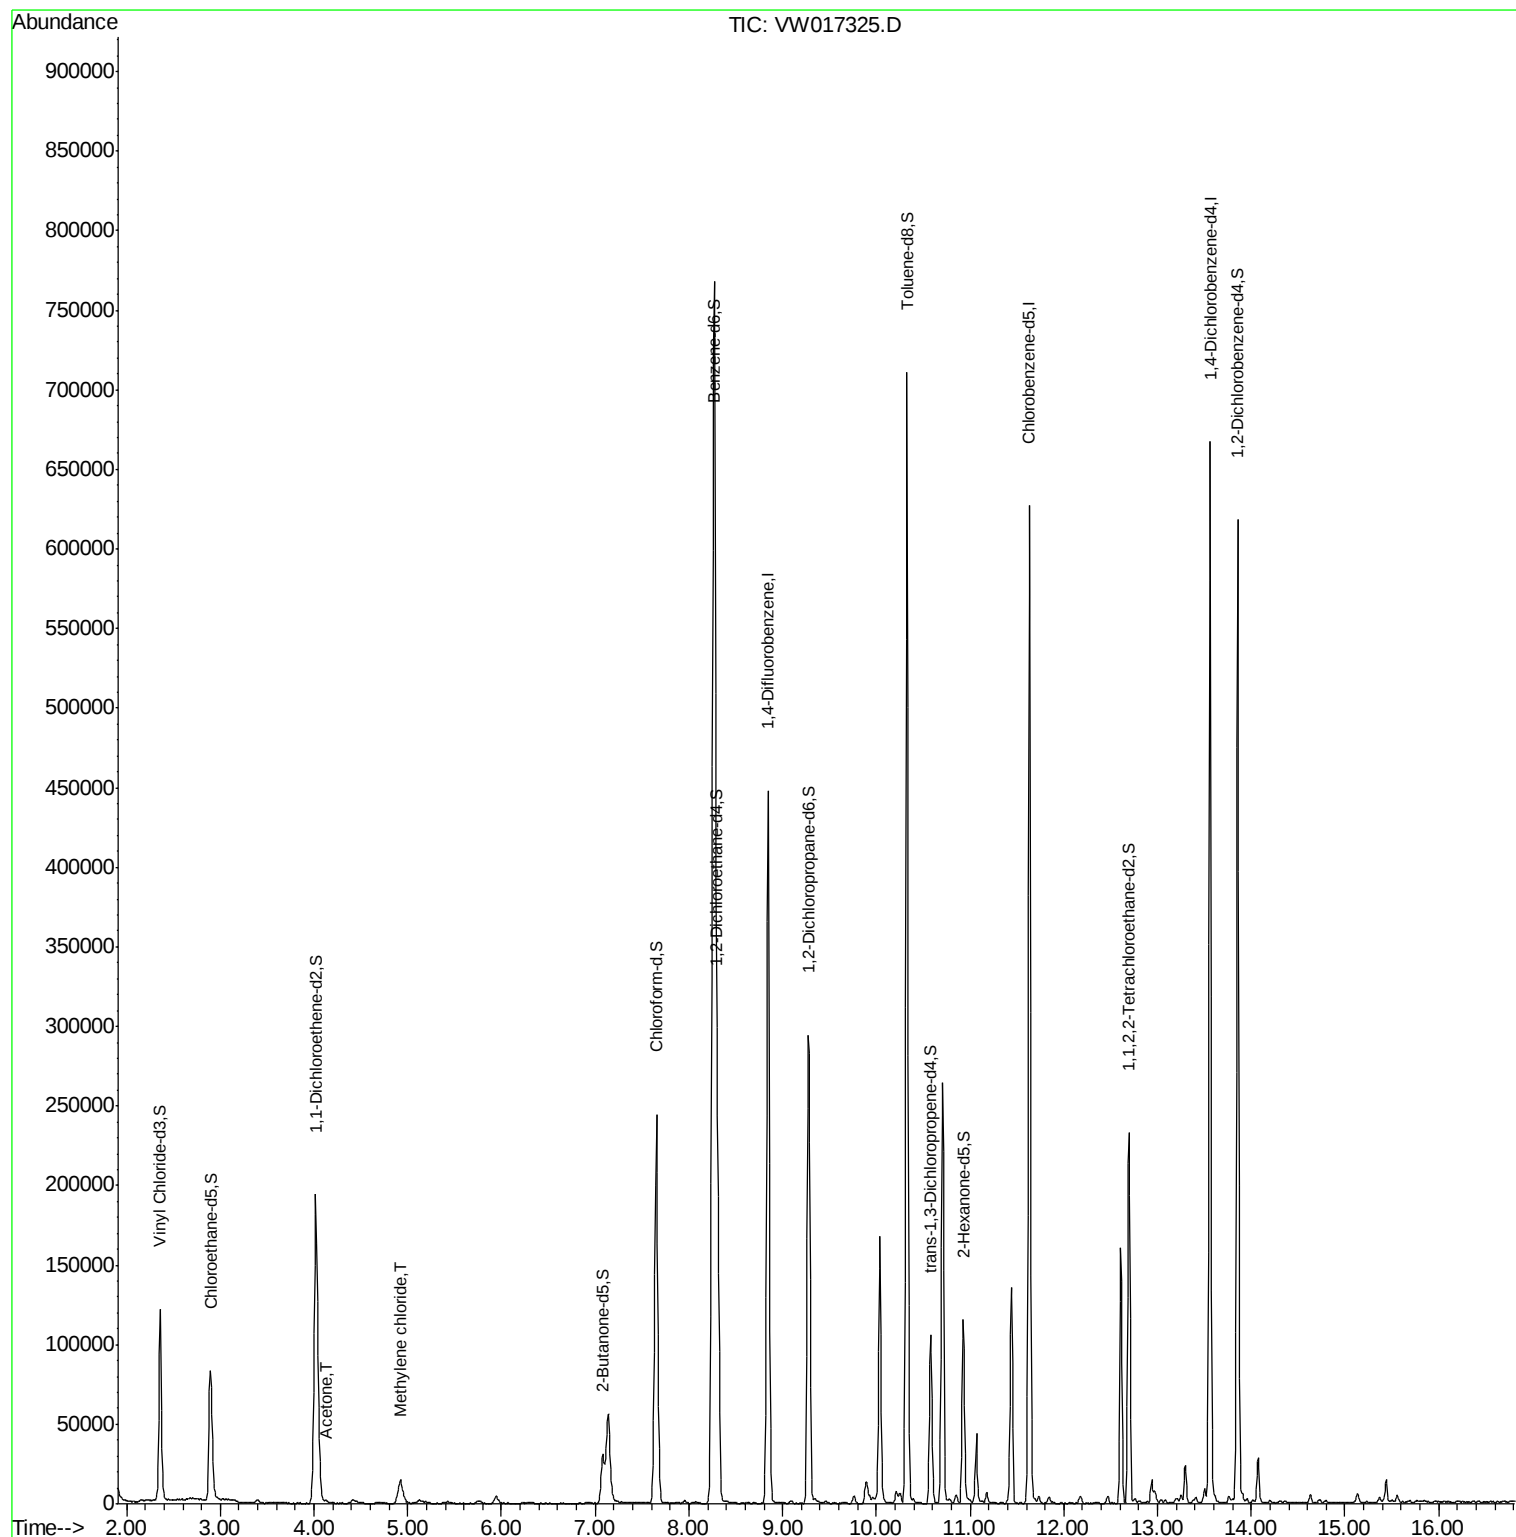

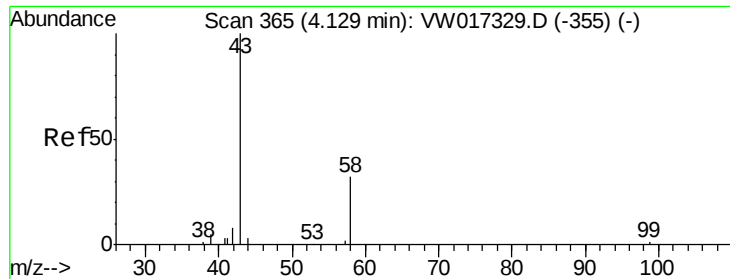

#13

Acetone

Concen: 2.521 ug/L

RT: 4.13 min Scan# 365

Delta R.T. -0.00 min

Lab File: VW017325.D

Acq: 18 Nov 2020 13:47

Instrument :

MSVOA_W

ClientSampled :





VIBLK

Tot Ion: 43 Resp: 1812

Ion Ratio Lower Upper

43 100

58 15.4 0.0 67.0

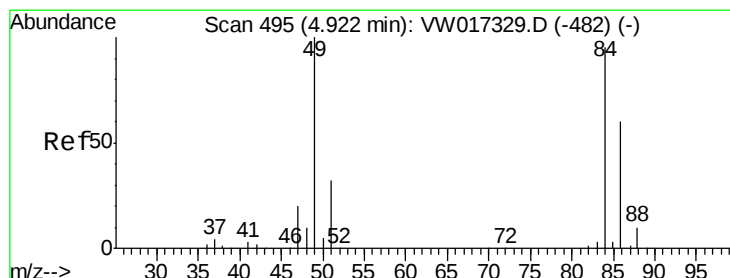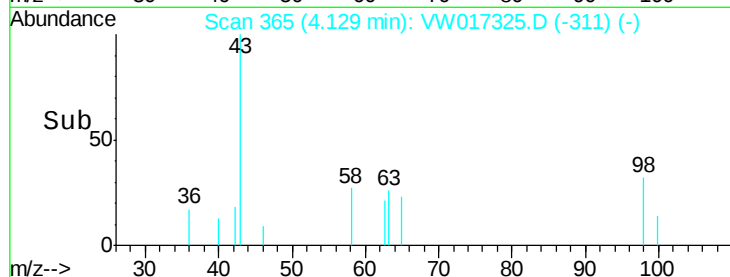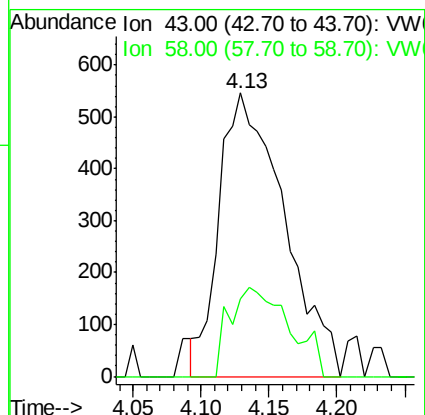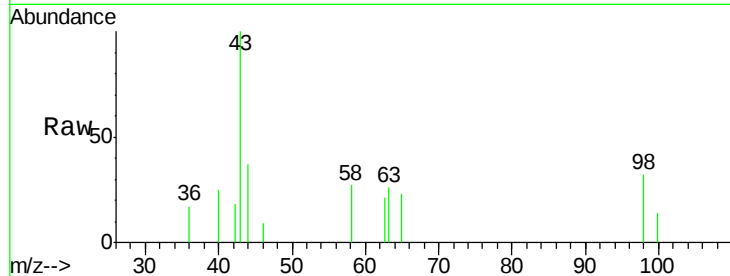

#16

Methylene chloride

Concen: 1.826 ug/L

RT: 4.92 min Scan# 495

Delta R.T. -0.00 min

Lab File: VW017325.D

Acq: 18 Nov 2020 13:47

Tgt Ion: 84 Resp: 12658

Ion Ratio Lower Upper

84 100

49 103.3 71.5 132.9

86 62.8 42.8 79.4

