

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111820\
 Data File : VW017347.D
 Acq On : 18 Nov 2020 22:59
 Operator : SY/VA
 Sample : L4749-15
 Misc : 5.58G/10ML/MSVOA W/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B14

Quant Time: Nov 19 06:24:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 19 05:03:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	359065	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	305641	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	116246	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	121322	22.82	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.28%
7) Chloroethane-d5	2.89	69	96333	22.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.24%
10) 1,1-Dichloroethene-d2	4.02	63	155944	16.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.08%
20) 2-Butanone-d5	7.08	46	38300	43.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.74%
24) Chloroform-d	7.65	84	216529	22.95	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	8.31	65	118265	25.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.80%
29) Benzene-d6	8.27	84	412635	23.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.80%
33) 1,2-Dichloropropane-d6	9.27	67	118141	25.74	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.96%
37) Toluene-d8	10.33	98	367890	22.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.72%
38) trans-1,3-Dichloropropene-	10.58	79	42511	21.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.08%
39) 2-Hexanone-d5	10.93	63	30249	49.15	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	94165	27.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.28%
61) 1,2-Dichlorobenzene-d4	13.86	152	105655	24.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.48%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	16815	2.738 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111820\
Data File : VW017347.D
Acq On : 18 Nov 2020 22:59
Operator : SY/VA
Sample : L4749-15
Misc : 5.58G/10ML/MSVOA W/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B14

Quant Time: Nov 19 06:24:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 19 05:03:18 2020
Response via : Initial Calibration

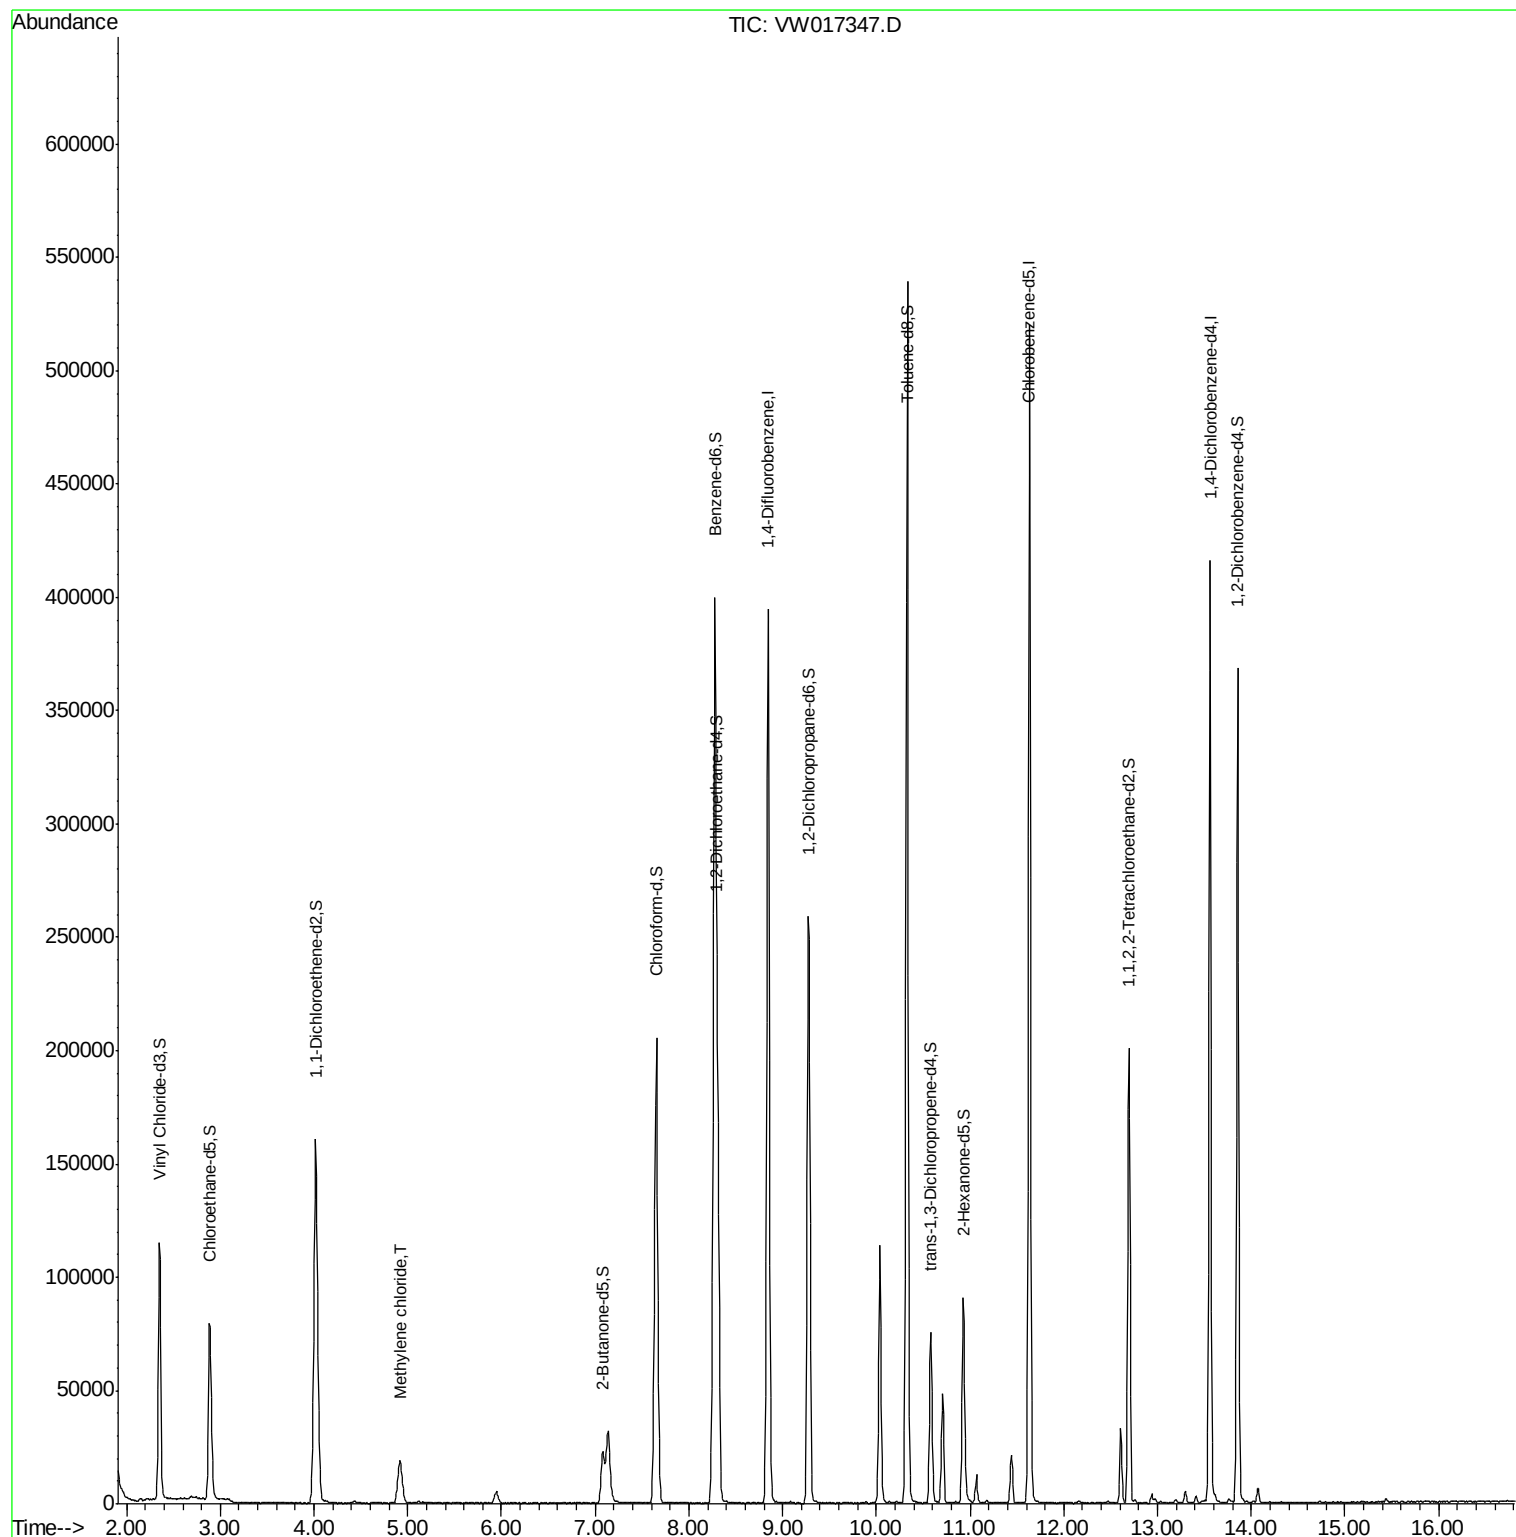

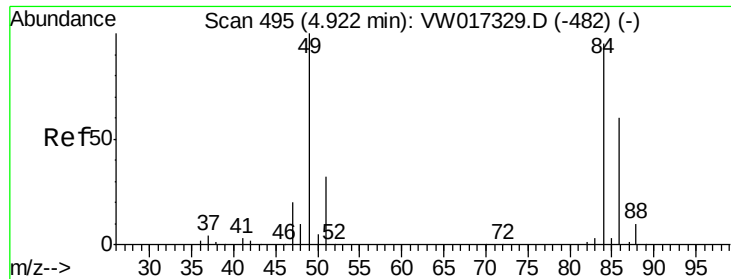

#16
 Methvlene chloride
 Concen: 2.738 ug/L
 RT: 4.92 min Scan# 494
 Delta R.T. -0.01 min
 Lab File: VW017347.D
 Acq: 18 Nov 2020 22:59

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B14

Tot Ion:	84	Resp:	16815
Ion	Ratio	Lower	Upper
84	100		
49	104.6	71.5	132.9
86	61.2	42.8	79.4

