

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111820\
 Data File : VW017353.D
 Acq On : 19 Nov 2020 01:20
 Operator : SY/VA
 Sample : L4749-22
 Misc : 5.58G/10ML/MSVOA W/SOIL
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG1

Quant Time: Nov 19 06:46:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 19 05:03:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	435601	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	365804	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	126021	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	145517	22.56	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.24%
7) Chloroethane-d5	2.89	69	118141	23.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.24%
10) 1,1-Dichloroethene-d2	4.02	63	191320	16.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.84%
20) 2-Butanone-d5	7.08	46	36090	34.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.16%
24) Chloroform-d	7.65	84	269792	23.58	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.32%
26) 1,2-Dichloroethane-d4	8.31	65	136324	24.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.60%
29) Benzene-d6	8.27	84	516658	25.05	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.20%
33) 1,2-Dichloropropane-d6	9.27	67	146757	26.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.84%
37) Toluene-d8	10.32	98	471038	24.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.04%
38) trans-1,3-Dichloropropene-	10.58	79	48558	20.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.20%
39) 2-Hexanone-d5	10.93	63	27918	37.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	101512	24.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	118109	25.39	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.56%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	16807	2.256 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111820\
Data File : VW017353.D
Acq On : 19 Nov 2020 01:20
Operator : SY/VA
Sample : L4749-22
Misc : 5.58G/10ML/MSVOA W/SOIL
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG1

Quant Time: Nov 19 06:46:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 19 05:03:18 2020
Response via : Initial Calibration

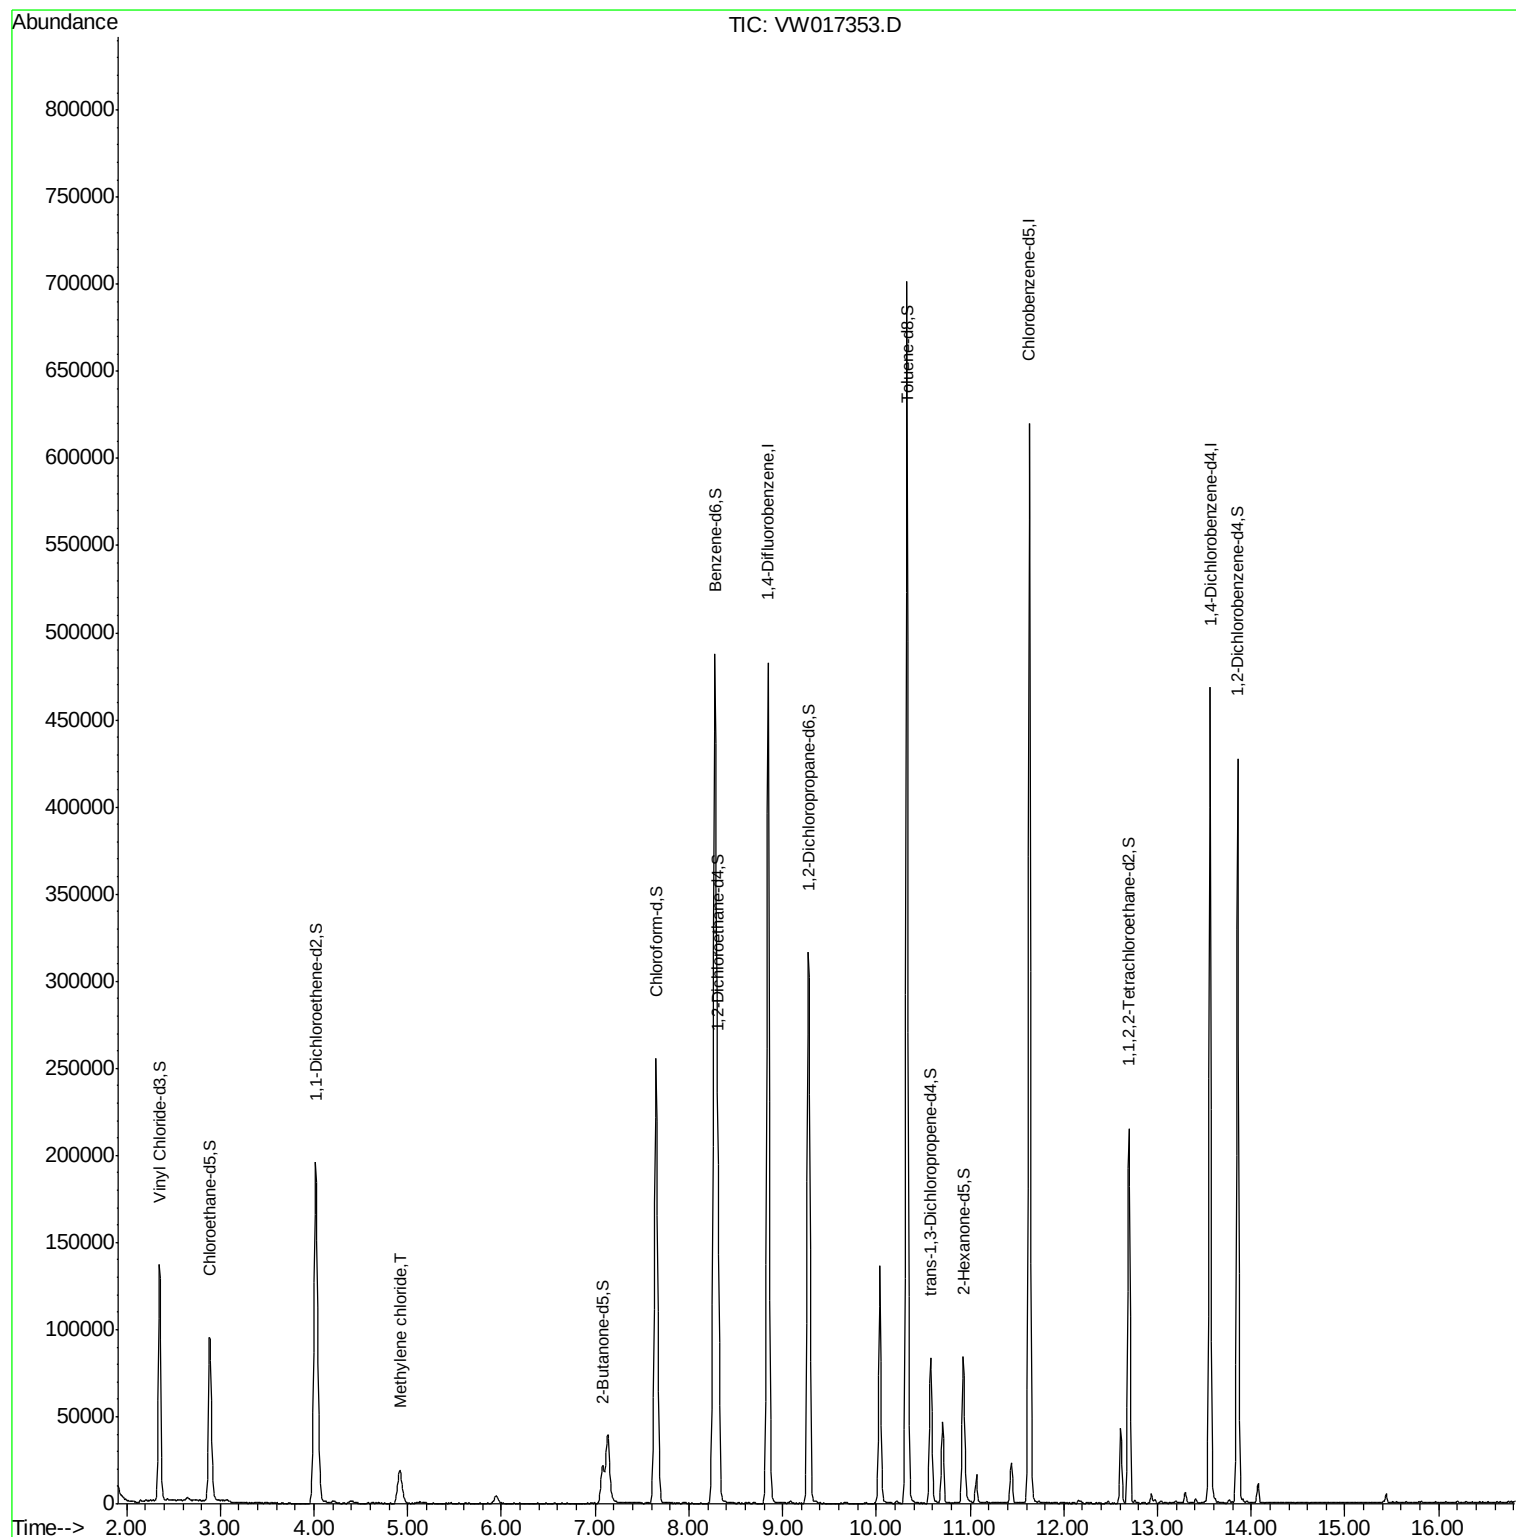

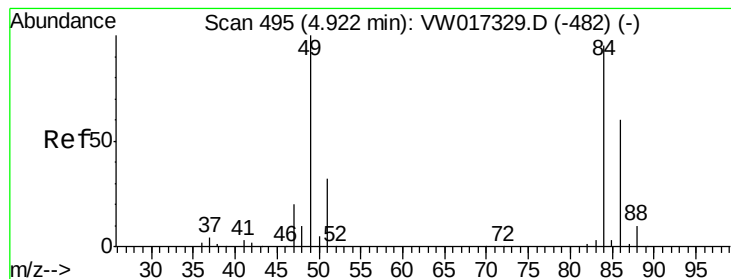

#16
 Methvlene chloride
 Concen: 2.256 ug/L
 RT: 4.92 min Scan# 494
 Delta R.T. -0.01 min
 Lab File: VW017353.D
 Acq: 19 Nov 2020 01:20

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG1

Tot Ion: 84 Resp: 16807
 Ion Ratio Lower Upper
 84 100
 49 100.4 71.5 132.9
 86 65.2 42.8 79.4

