

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111820\
 Data File : VW017354.D
 Acq On : 19 Nov 2020 01:43
 Operator : SY/VA
 Sample : L4751-08
 Misc : 5.63G/10ML/MSVOA W/SOIL
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG2

Quant Time: Nov 19 06:49:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 19 05:03:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	435042	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	337688	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	105638	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	161406	25.06	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.24%
7) Chloroethane-d5	2.89	69	129016	25.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.88%
10) 1,1-Dichloroethene-d2	4.02	63	207029	18.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.52%
20) 2-Butanone-d5	7.08	46	24118	22.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.60%
24) Chloroform-d	7.65	84	279672	24.47	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.88%
26) 1,2-Dichloroethane-d4	8.30	65	130702	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.68%
29) Benzene-d6	8.27	84	539090	28.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.28%
33) 1,2-Dichloropropane-d6	9.27	67	148589	29.30	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	117.20%
37) Toluene-d8	10.33	98	483598	26.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.92%
38) trans-1,3-Dichloropropene-	10.58	79	40024	18.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.52%
39) 2-Hexanone-d5	10.93	63	18480	27.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	86944	22.62	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	98926	25.37	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.48%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	16756	2.252 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111820\
Data File : VW017354.D
Acq On : 19 Nov 2020 01:43
Operator : SY/VA
Sample : L4751-08
Misc : 5.63G/10ML/MSVOA W/SOIL
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG2

Quant Time: Nov 19 06:49:19 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 19 05:03:18 2020
Response via : Initial Calibration

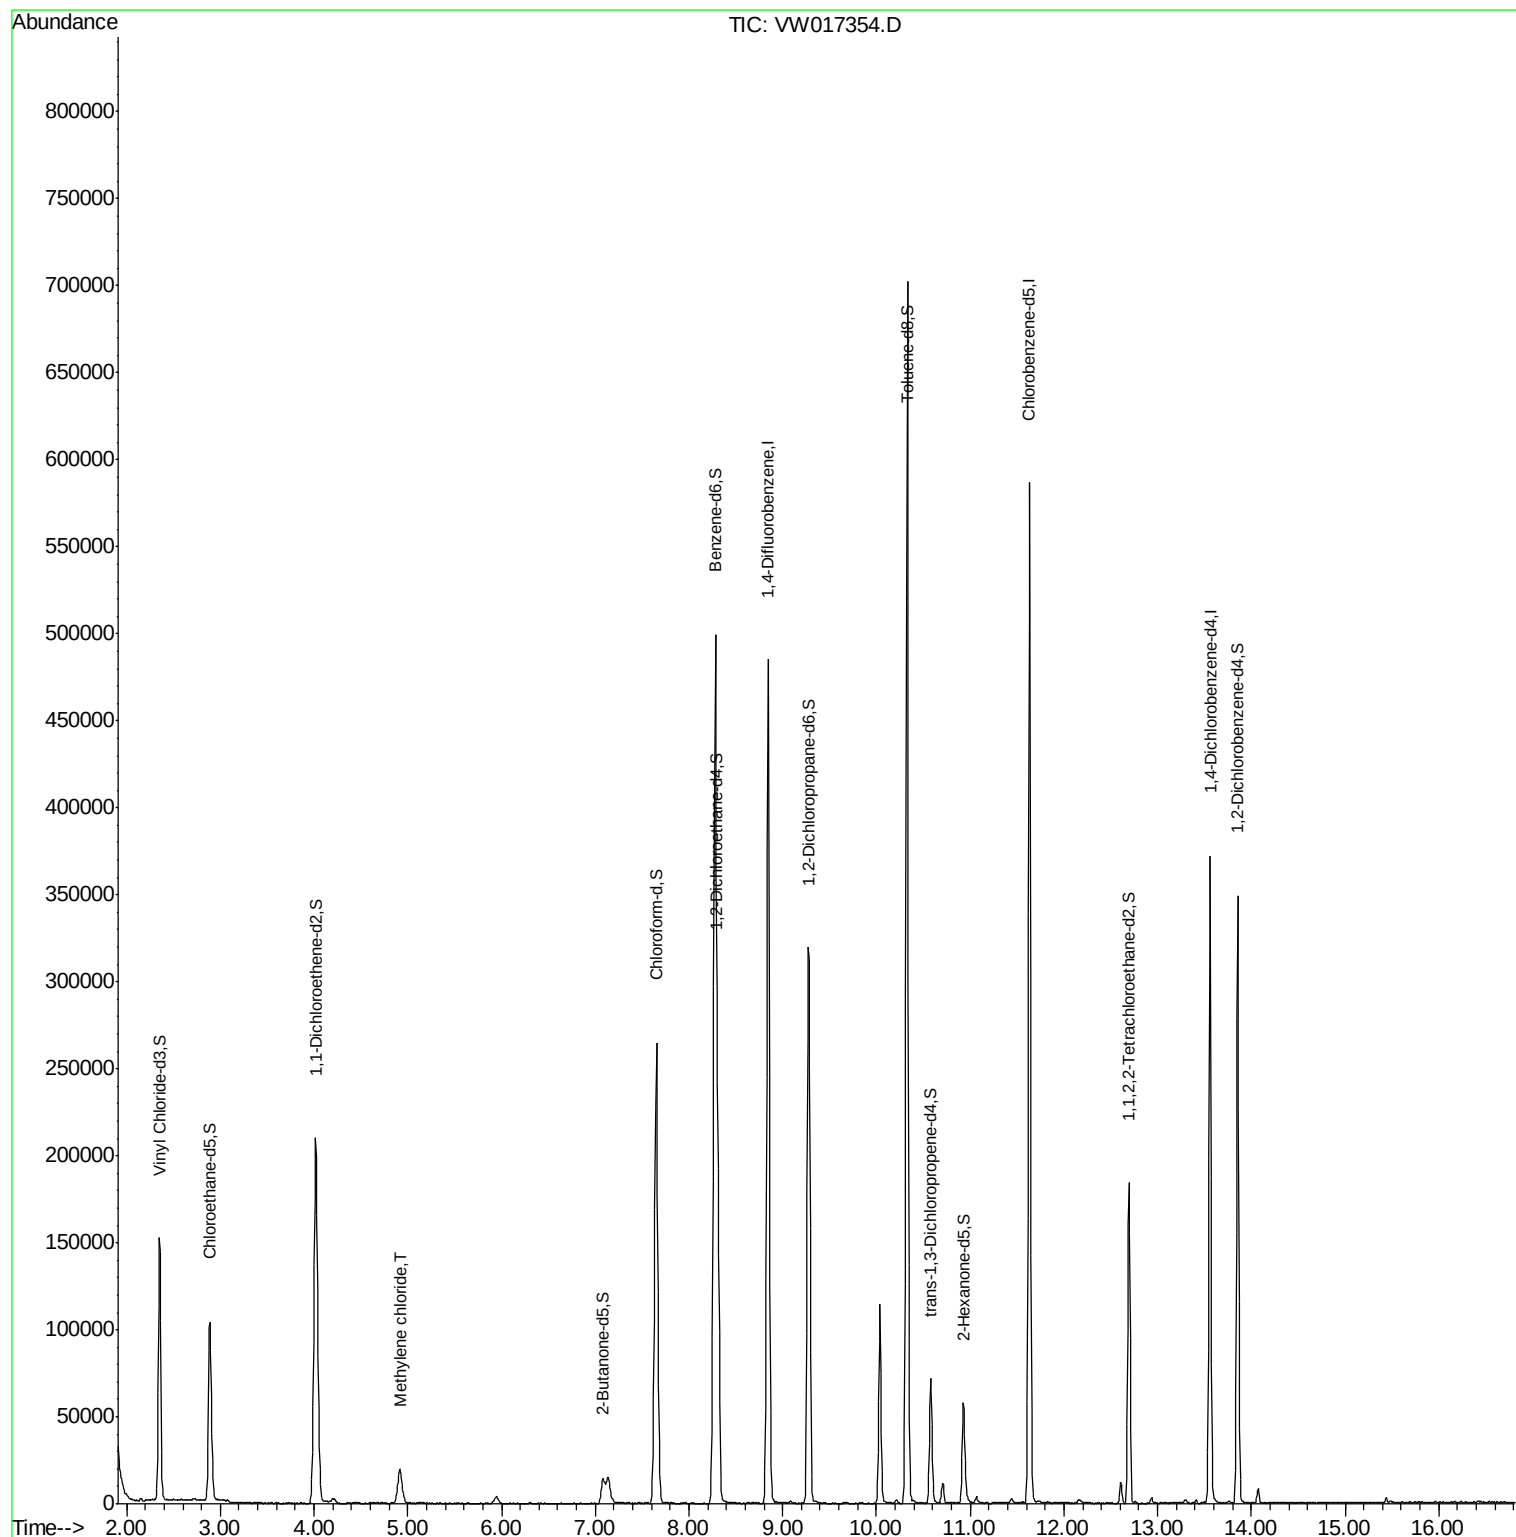

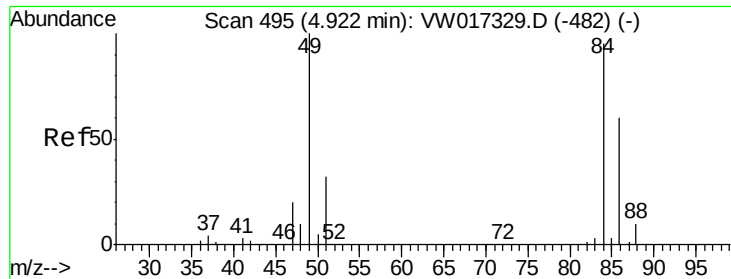

#16
 Methvlene chloride
 Concen: 2.252 ug/L
 RT: 4.92 min Scan# 495
 Delta R.T. -0.00 min
 Lab File: VW017354.D
 Acq: 19 Nov 2020 01:43

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG2

Tot Ion: 84 Resp: 16756
 Ion Ratio Lower Upper
 84 100
 49 101.6 71.5 132.9
 86 61.1 42.8 79.4

