

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
 Data File : VW031040.D
 Acq On : 18 Nov 2024 12:29
 Operator : SY/MD
 Sample : VW1118SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 19 00:29:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 19 00:28:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	341171	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	332814	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	152568	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	59127	10.567	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.280%
7) Chloroethane-d5	2.899	69	54411	12.679	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.720%
11) 1,1-Dichloroethene-d2	4.021	65	32300	13.990	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.960%
21) 2-Butanone-d5	7.075	46	43052	46.754	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.500%
24) Chloroform-d	7.648	84	183982	18.292	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.160%
26) 1,2-Dichloroethane-d4	8.300	65	96849	19.367	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.480%
32) Benzene-d6	8.270	84	347835	16.823	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	67.280%
36) 1,2-Dichloropropane-d6	9.270	67	110768	18.173	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	72.680%
41) Toluene-d8	10.318	98	302839	16.329	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.320%
43) trans-1,3-Dichloroprop...	10.574	79	42142	17.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.240%
47) 2-Hexanone-d5	10.922	63	35009	44.319	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94061	22.150	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	115526	20.788	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.160%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	2975	0.371	ug/L	Qvalue # 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031040.D
Acq On : 18 Nov 2024 12:29
Operator : SY/MD
Sample : VW1118SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 19 00:29:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

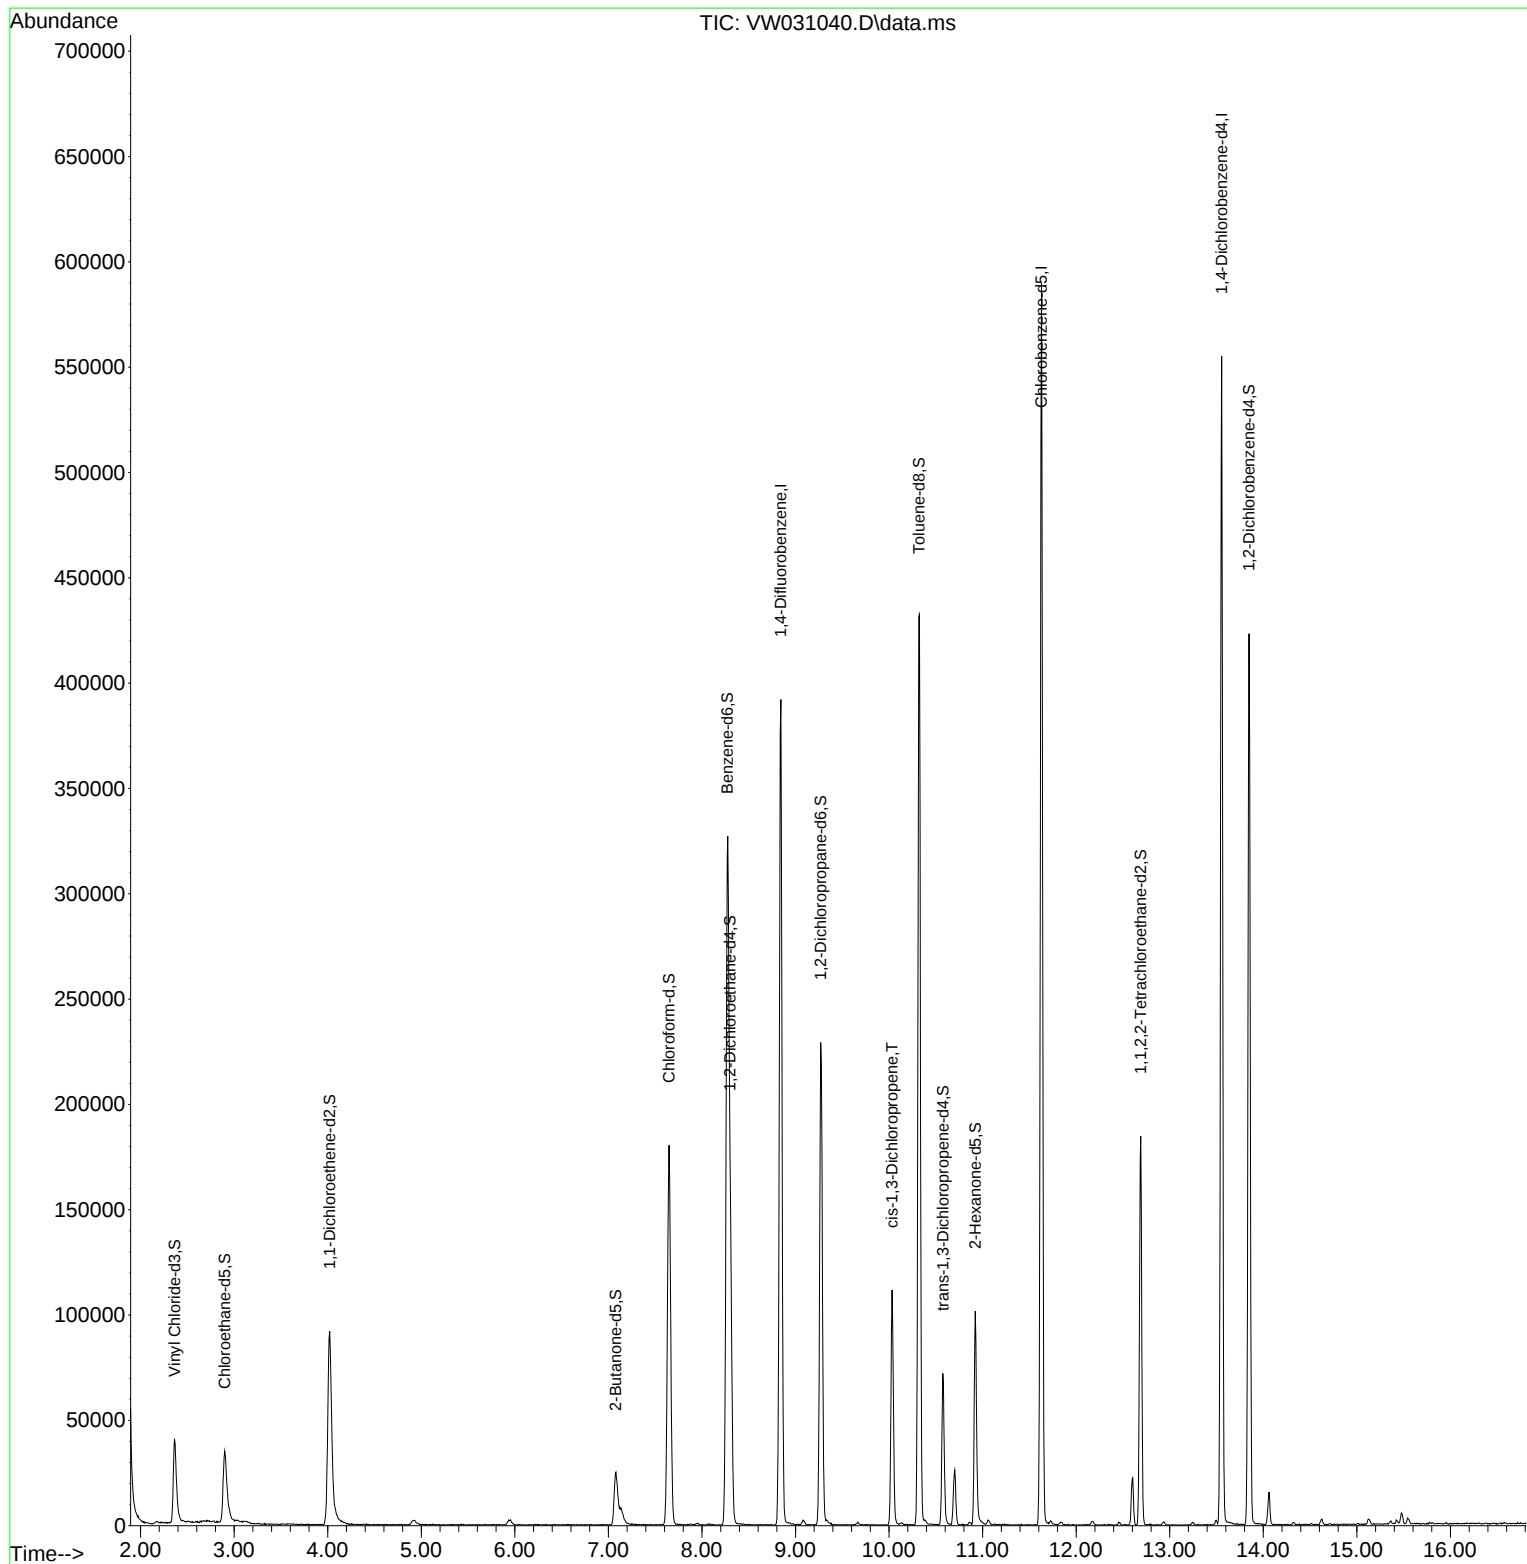

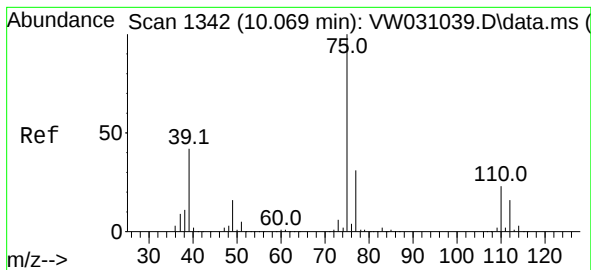

#39
 cis-1,3-Dichloropropene
 Concen: 0.371 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW031040.D
 Acq: 18 Nov 2024 12:29

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2975
 Ion Ratio Lower Upper
 75 100
 77 53.6 21.3 39.6#

