




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031046.D
Acq On : 18 Nov 2024 16:01
Operator : SY/MD
Sample : P4872-18
Misc : 5.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/19/2024
Supervised By :Semsettin Yesilyurt 11/19/2024

Quant Time: Nov 19 00:30:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

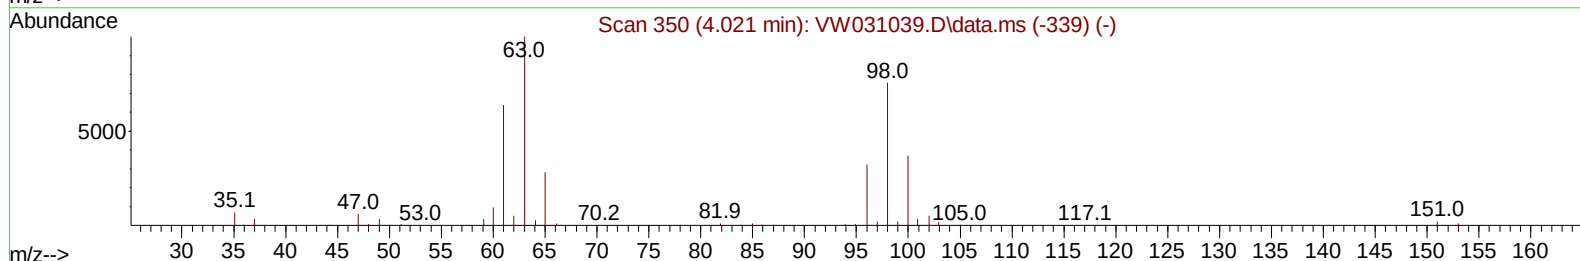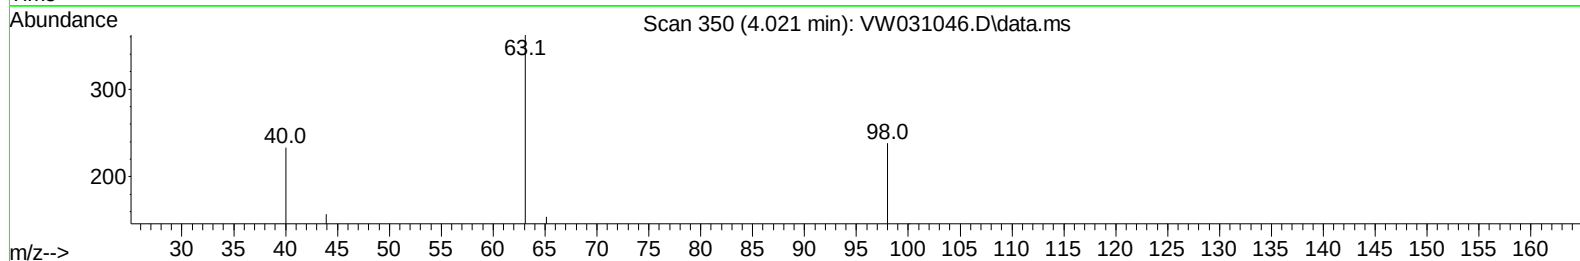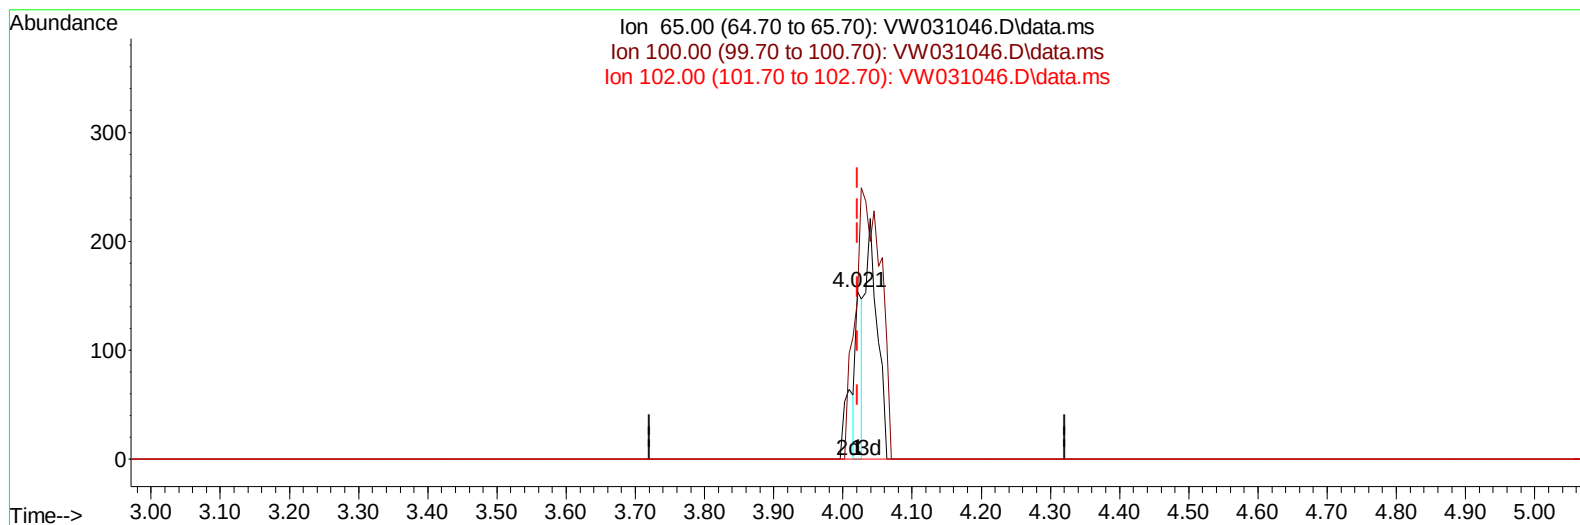

TIC: VW031046.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.000) 4.26 ug/L

response 110

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	134.90	346.36#
102.00	20.20	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031046.D
Acq On : 18 Nov 2024 16:01
Operator : SY/MD
Sample : P4872-18
Misc : 5.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:30:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/19/2024
Supervised By :Semsettin Yesilyurt 11/19/2024

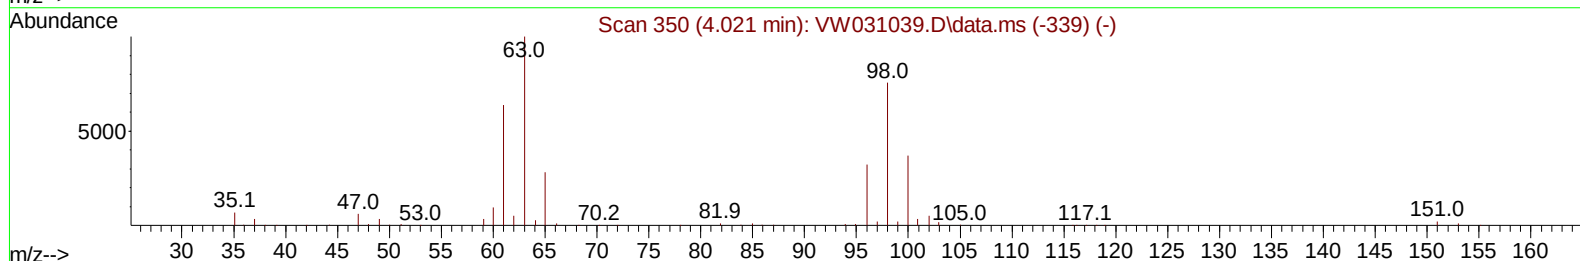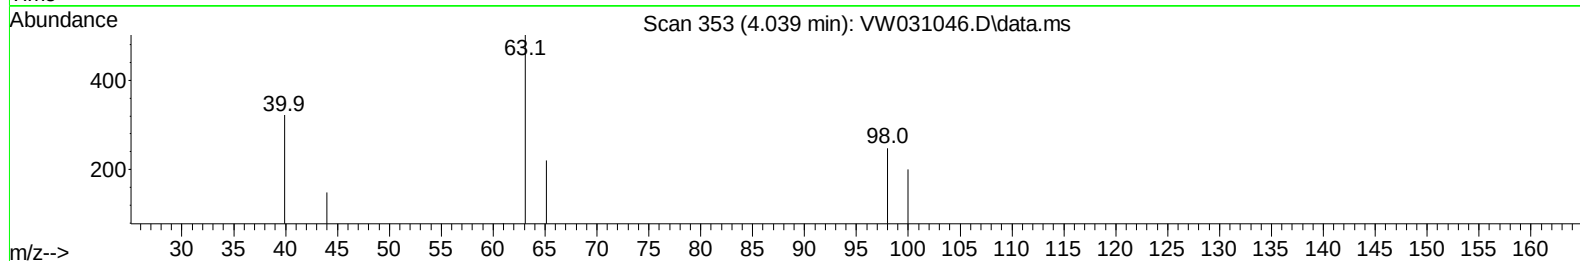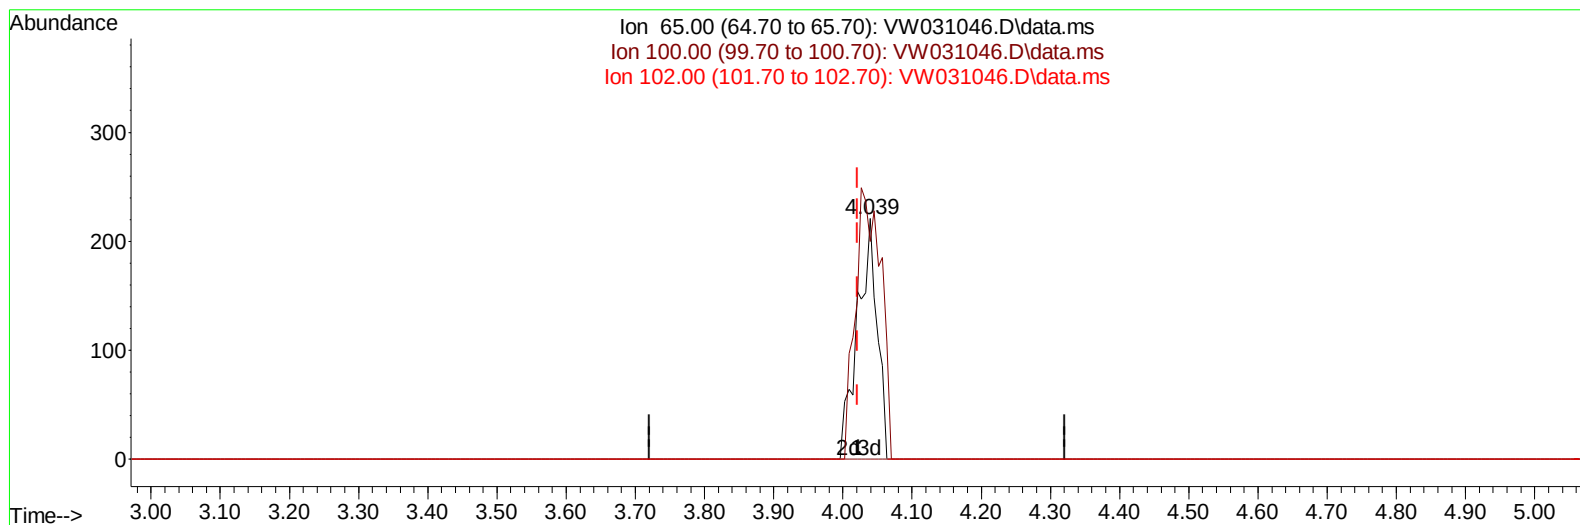

TIC: VW031046.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.039min (+ 0.018) 16.87 ug/L m

response 436

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	134.90	87.39#
102.00	20.20	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031046.D
Acq On : 18 Nov 2024 16:01
Operator : SY/MD
Sample : P4872-18
Misc : 5.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:30:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/19/2024
Supervised By :Semsettin Yesilyurt 11/19/2024

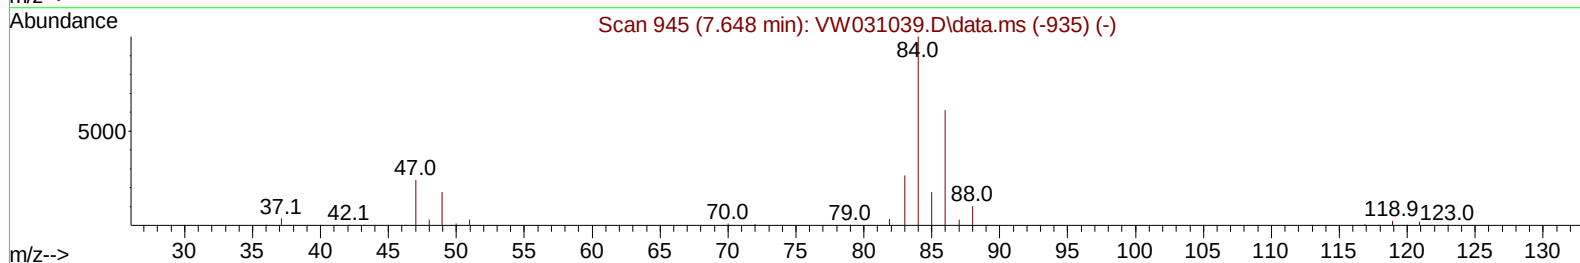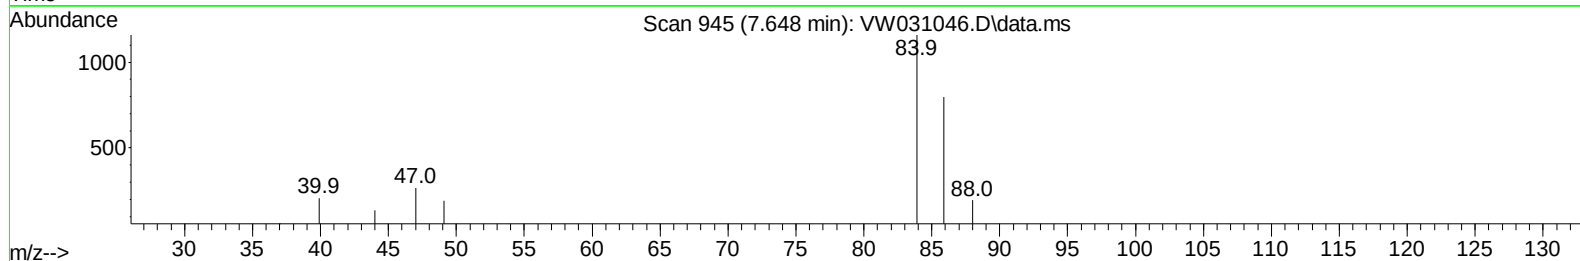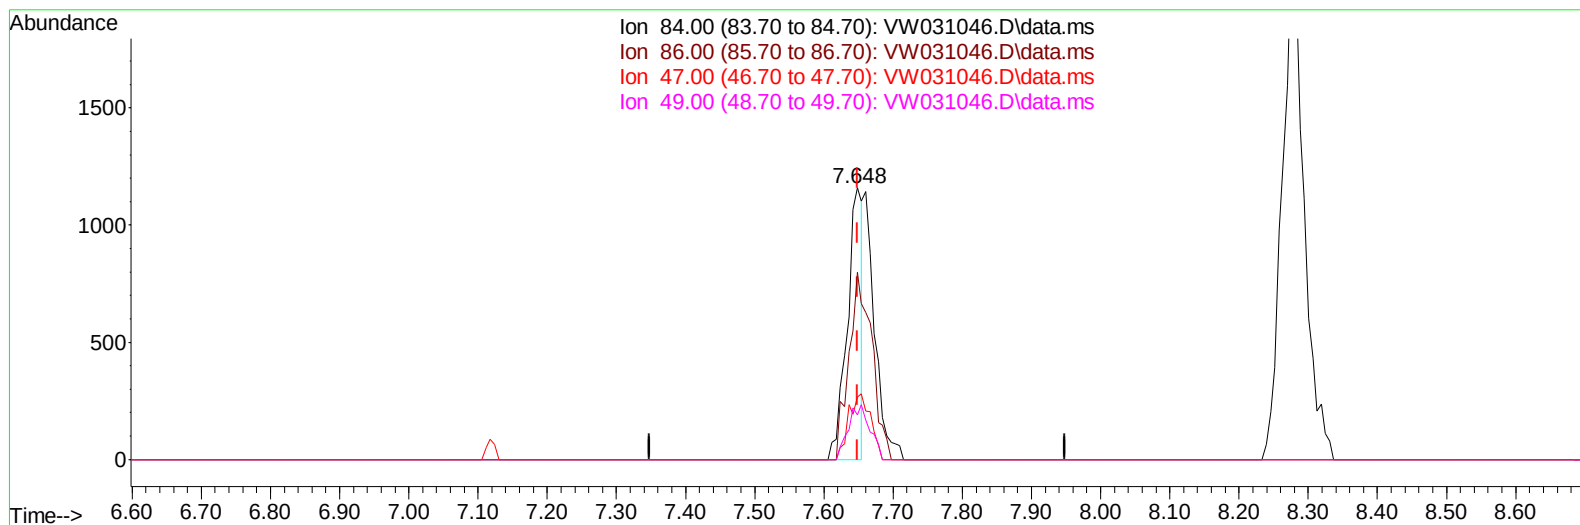

TIC: VW031046.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 15.75 ug/L

response 1773

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.60	103.38#
47.00	41.30	34.69
49.00	24.80	28.37




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031046.D
Acq On : 18 Nov 2024 16:01
Operator : SY/MD
Sample : P4872-18
Misc : 5.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:30:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/19/2024
Supervised By :Semsettin Yesilyurt 11/19/2024

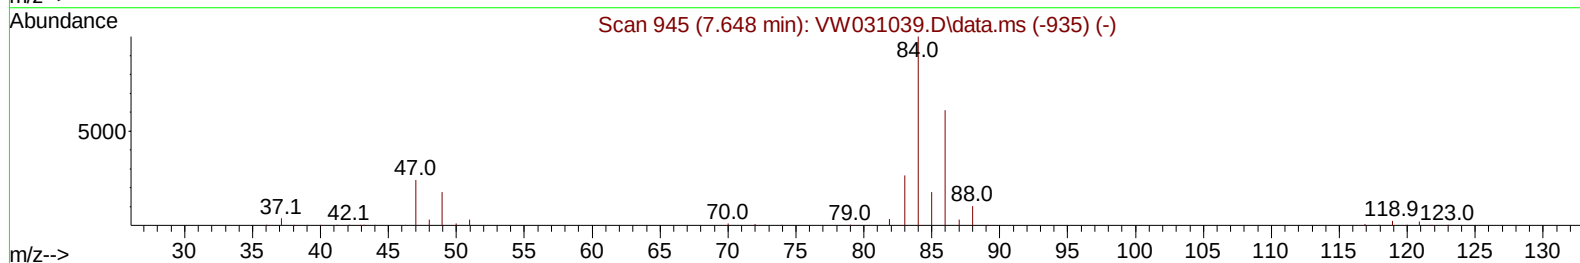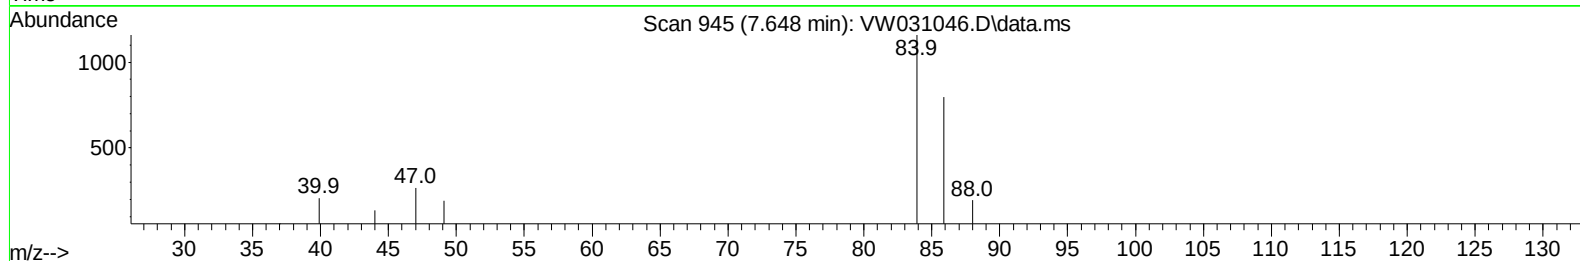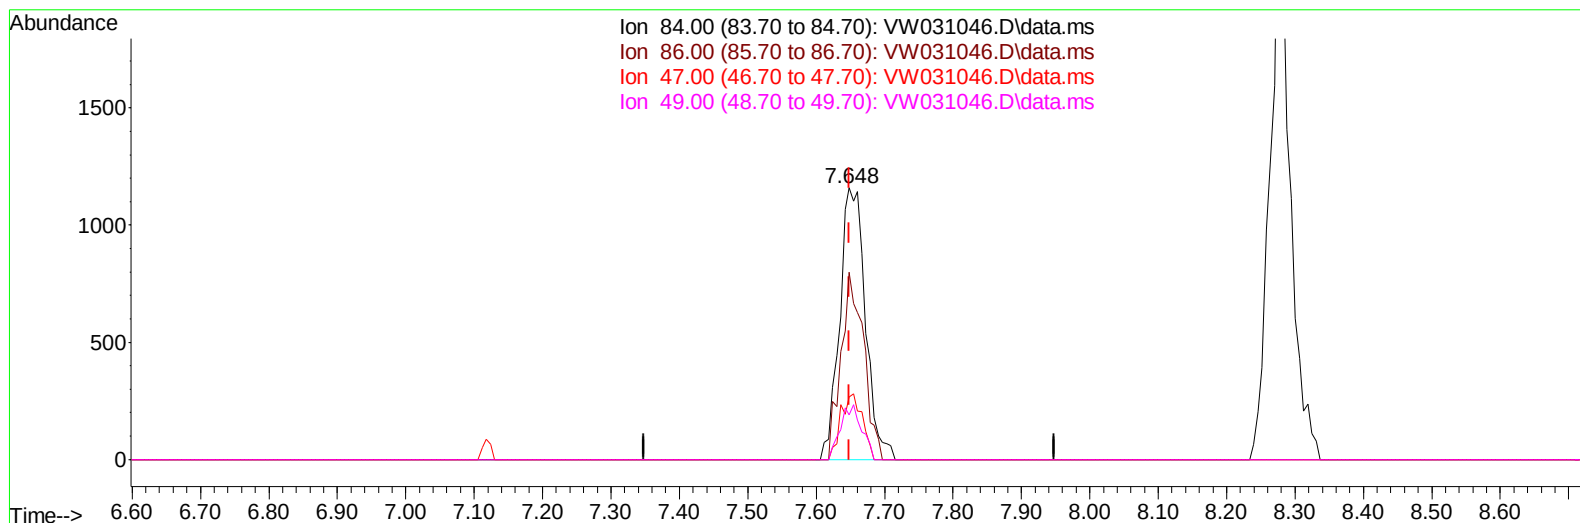

TIC: VW031046.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 26.97 ug/L m

response 3036

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.60	60.38
47.00	41.30	20.26#
49.00	24.80	16.57#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw111824\
 Data File : VW031046.D
 Acq On : 18 Nov 2024 16:01
 Operator : SY/MD
 Sample : P4872-18
 Misc : 5.77g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:30:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 19 00:28:30 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/19/2024
 Supervised By :Semsettin Yesilyurt 11/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.849	114		3819	25.000	ug/L	0.01
28) Chlorobenzene-d5	11.629	117		3416	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		1028	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		964	15.391	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	61.560%		
7) Chloroethane-d5	2.905	69		1016	21.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	84.600%		
11) 1,1-Dichloroethene-d2	4.039	65		436m	16.870	ug/L	0.02
Spiked Amount 25.000	Range 45	- 110		Recovery =	67.480%		
21) 2-Butanone-d5	0.000	46		0d	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.000%#		
24) Chloroform-d	7.648	84		3036m	26.966	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	107.880%		
26) 1,2-Dichloroethane-d4	8.313	65		1670	29.833	ug/L	0.01
Spiked Amount 25.000	Range 70	- 130		Recovery =	119.320%		
32) Benzene-d6	8.276	84		4845	22.830	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	91.320%		
36) 1,2-Dichloropropane-d6	9.276	67		1914	30.594	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	122.360%#		
41) Toluene-d8	10.331	98		3563	18.718	ug/L	0.01
Spiked Amount 25.000	Range 30	- 130		Recovery =	74.880%		
43) trans-1,3-Dichloroprop...	10.581	79		220	8.676	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	34.720%		
47) 2-Hexanone-d5	0.000	63		0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.000%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		1585	36.365	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	145.440%#		
66) 1,2-Dichlorobenzene-d4	13.854	152		870	23.233	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	92.920%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031046.D
Acq On : 18 Nov 2024 16:01
Operator : SY/MD
Sample : P4872-18
Misc : 5.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:30:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/19/2024
Supervised By :Semsettin Yesilyurt 11/19/2024

