

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
 Data File : VW031044.D
 Acq On : 18 Nov 2024 15:13
 Operator : SY/MD
 Sample : P4872-16
 Misc : 6.36g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y3

Quant Time: Nov 19 00:30:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 19 00:28:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	95794	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	78977	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	23296	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	27588	17.560	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.240%
7) Chloroethane-d5	2.899	69	25815	21.424	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.680%
11) 1,1-Dichloroethene-d2	4.033	65	12707	19.601	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.400%
21) 2-Butanone-d5	7.081	46	19022	73.572	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.140%#
24) Chloroform-d	7.654	84	68137	24.128	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.520%
26) 1,2-Dichloroethane-d4	8.307	65	37144	26.454	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.800%
32) Benzene-d6	8.276	84	117173	23.882	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.520%
36) 1,2-Dichloropropane-d6	9.276	67	40407	27.937	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.760%
41) Toluene-d8	10.325	98	85314	19.386	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.560%
43) trans-1,3-Dichloroprop...	10.575	79	12370	21.099	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.400%
47) 2-Hexanone-d5	10.922	63	11782	62.853	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	36956	36.673	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	146.680%#
66) 1,2-Dichlorobenzene-d4	13.854	152	19781	23.311	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.240%
Target Compounds					Qvalue	
13) Acetone	4.131	43	26149	82.808	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031044.D
Acq On : 18 Nov 2024 15:13
Operator : SY/MD
Sample : P4872-16
Misc : 6.36g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y3


Quant Time: Nov 19 00:30:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

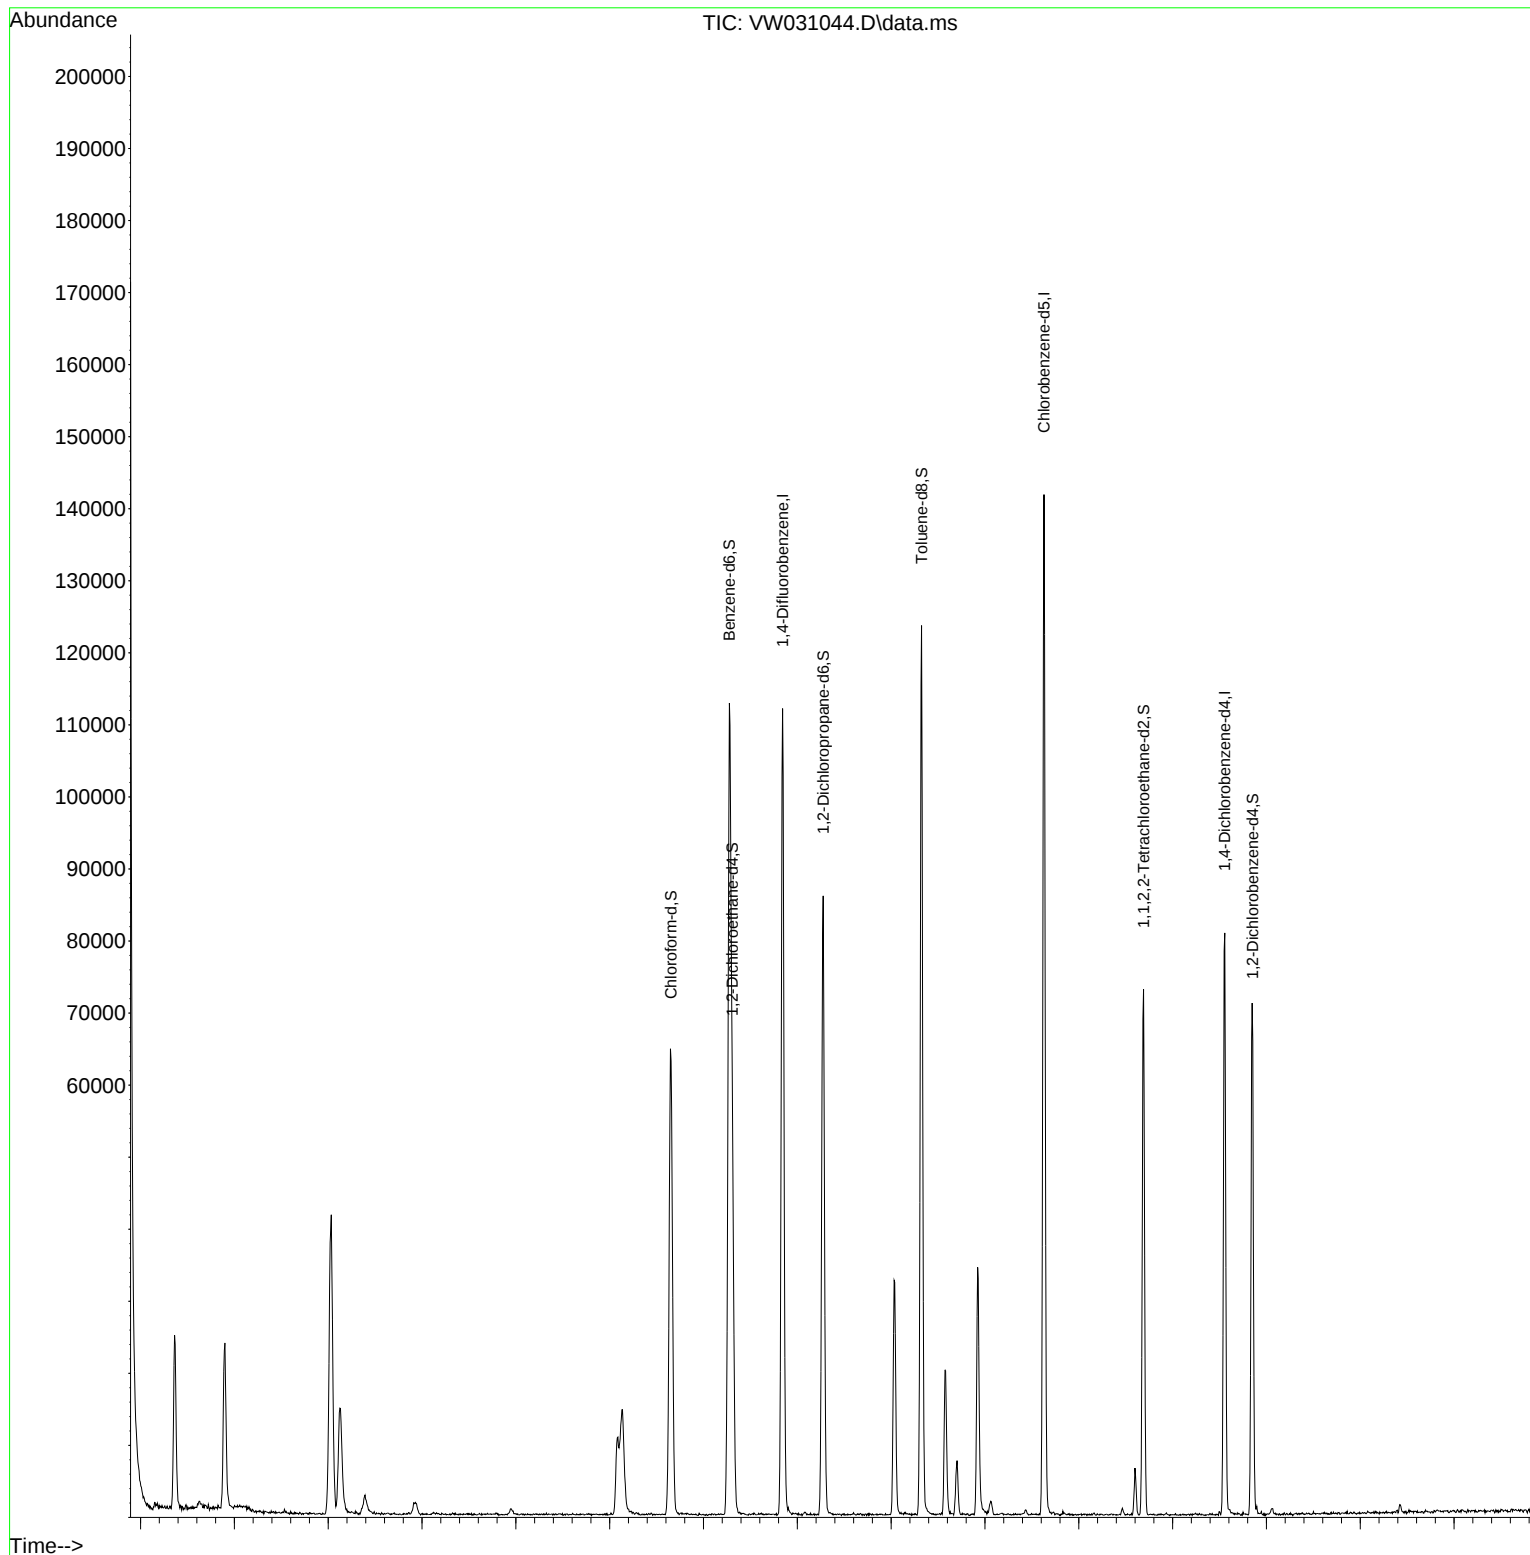

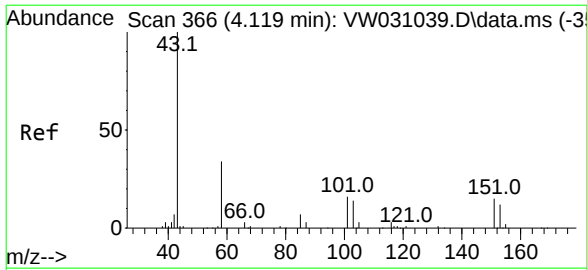

#13
 Acetone
 Concen: 82.808 ug/L
 RT: 4.131 min Scan# 368
 Delta R.T. 0.012 min
 Lab File: VW031044.D
 Acq: 18 Nov 2024 15:13

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y3

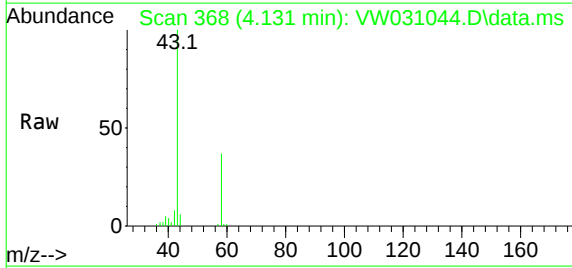

Tgt Ion: 43 Resp: 26149
 Ion Ratio Lower Upper
 43 100
 58 35.8 0.0 62.6

